

Sample Name :N-Formyl-Met-Leu-Phe
 Cat. No. : RP12956
 Lot. No. : PE8631902
 Time Processed : 9:06:12
 Month-Day-Year Processed : 03/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

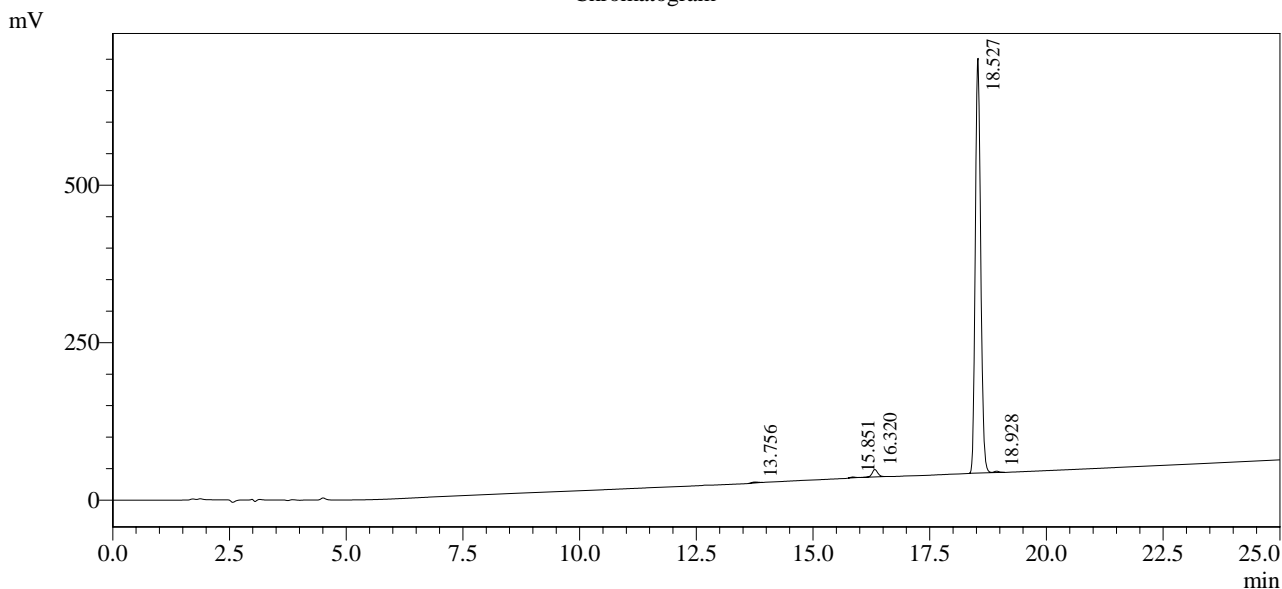

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.756	14045	1470	0.257
2	15.851	10085	1344	0.185
3	16.320	100317	11919	1.839
4	18.527	5314410	658599	97.407
5	18.928	17035	2237	0.312
Total		5455892	675569	100.000