

Sample Name :Uty HY Peptide (246-254)
 Cat. No. : RP20261
 Lot. No. : E4010819K
 Time Processed :8:29:22
 Month-Day-Year Processed : 12/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0286

Chromatogram

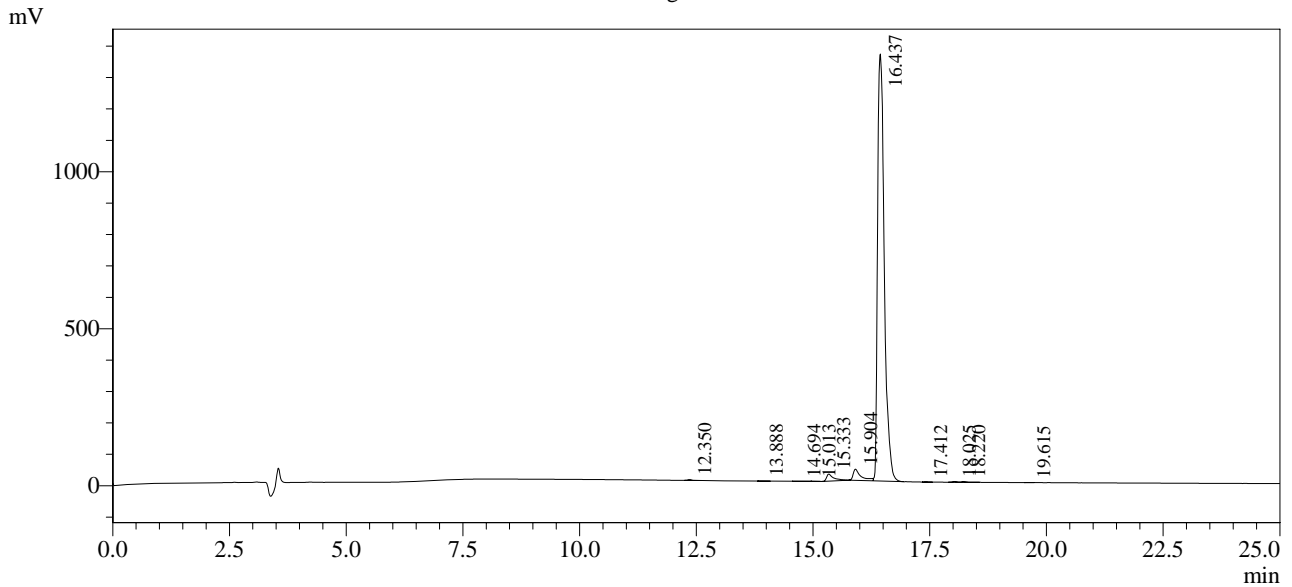

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.350	15065	2515	0.105
2	13.888	2258	328	0.016
3	14.694	3679	342	0.026
4	15.013	1492	151	0.010
5	15.333	236948	22318	1.658
6	15.904	415090	35844	2.904
7	16.437	13589789	1360267	95.069
8	17.412	1073	201	0.008
9	18.025	13840	1974	0.097
10	18.220	14318	1965	0.100
11	19.615	1037	175	0.007
Total		14294587	1426080	100.000