

Sample Name :Cys-TAT(47-57)  
 Cat No: RP20343  
 Lot No : E9348521H  
 Time Processed :9:58:25  
 Month-Day-Year Processed :08/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010140

### <Chromatogram>

mV

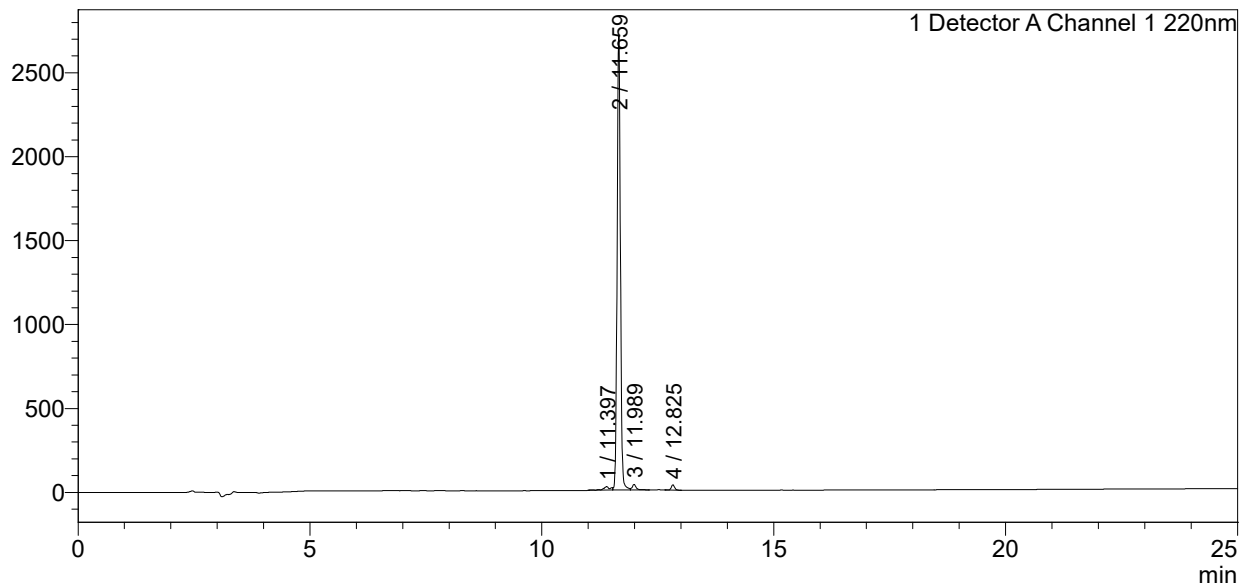

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.397	225993	21187	1.610
2	11.659	13464111	2707910	95.937
3	11.989	193985	33300	1.382
4	12.825	150269	31295	1.071
Total		14034359	2793692	100.000