

Sample Name :c-Myc Peptide  
 Cat No. : RP11731  
 Lot No. : E0683121A  
 Time Processed :7:59:21 AM  
 Month-Day-Year Processed :01/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ17010508

### <Chromatogram>

mV

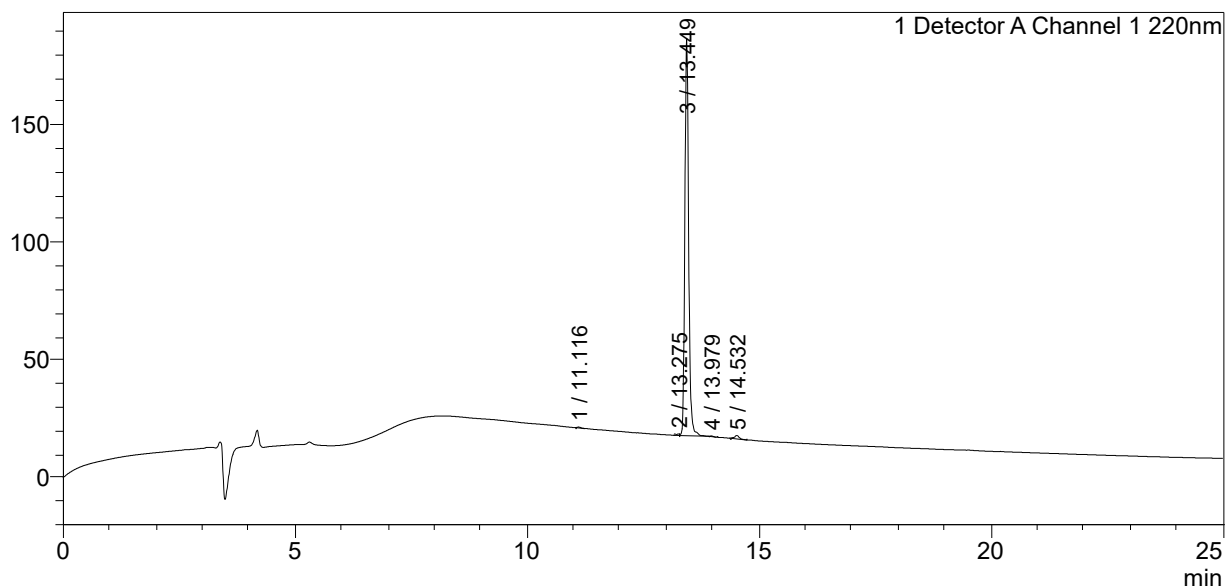

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.116	1749	362	0.178
2	13.275	3010	579	0.307
3	13.449	963434	169010	98.302
4	13.979	1429	288	0.146
5	14.532	10450	1501	1.066
Total		980072	171740	100.000