


# Mass Spectrum

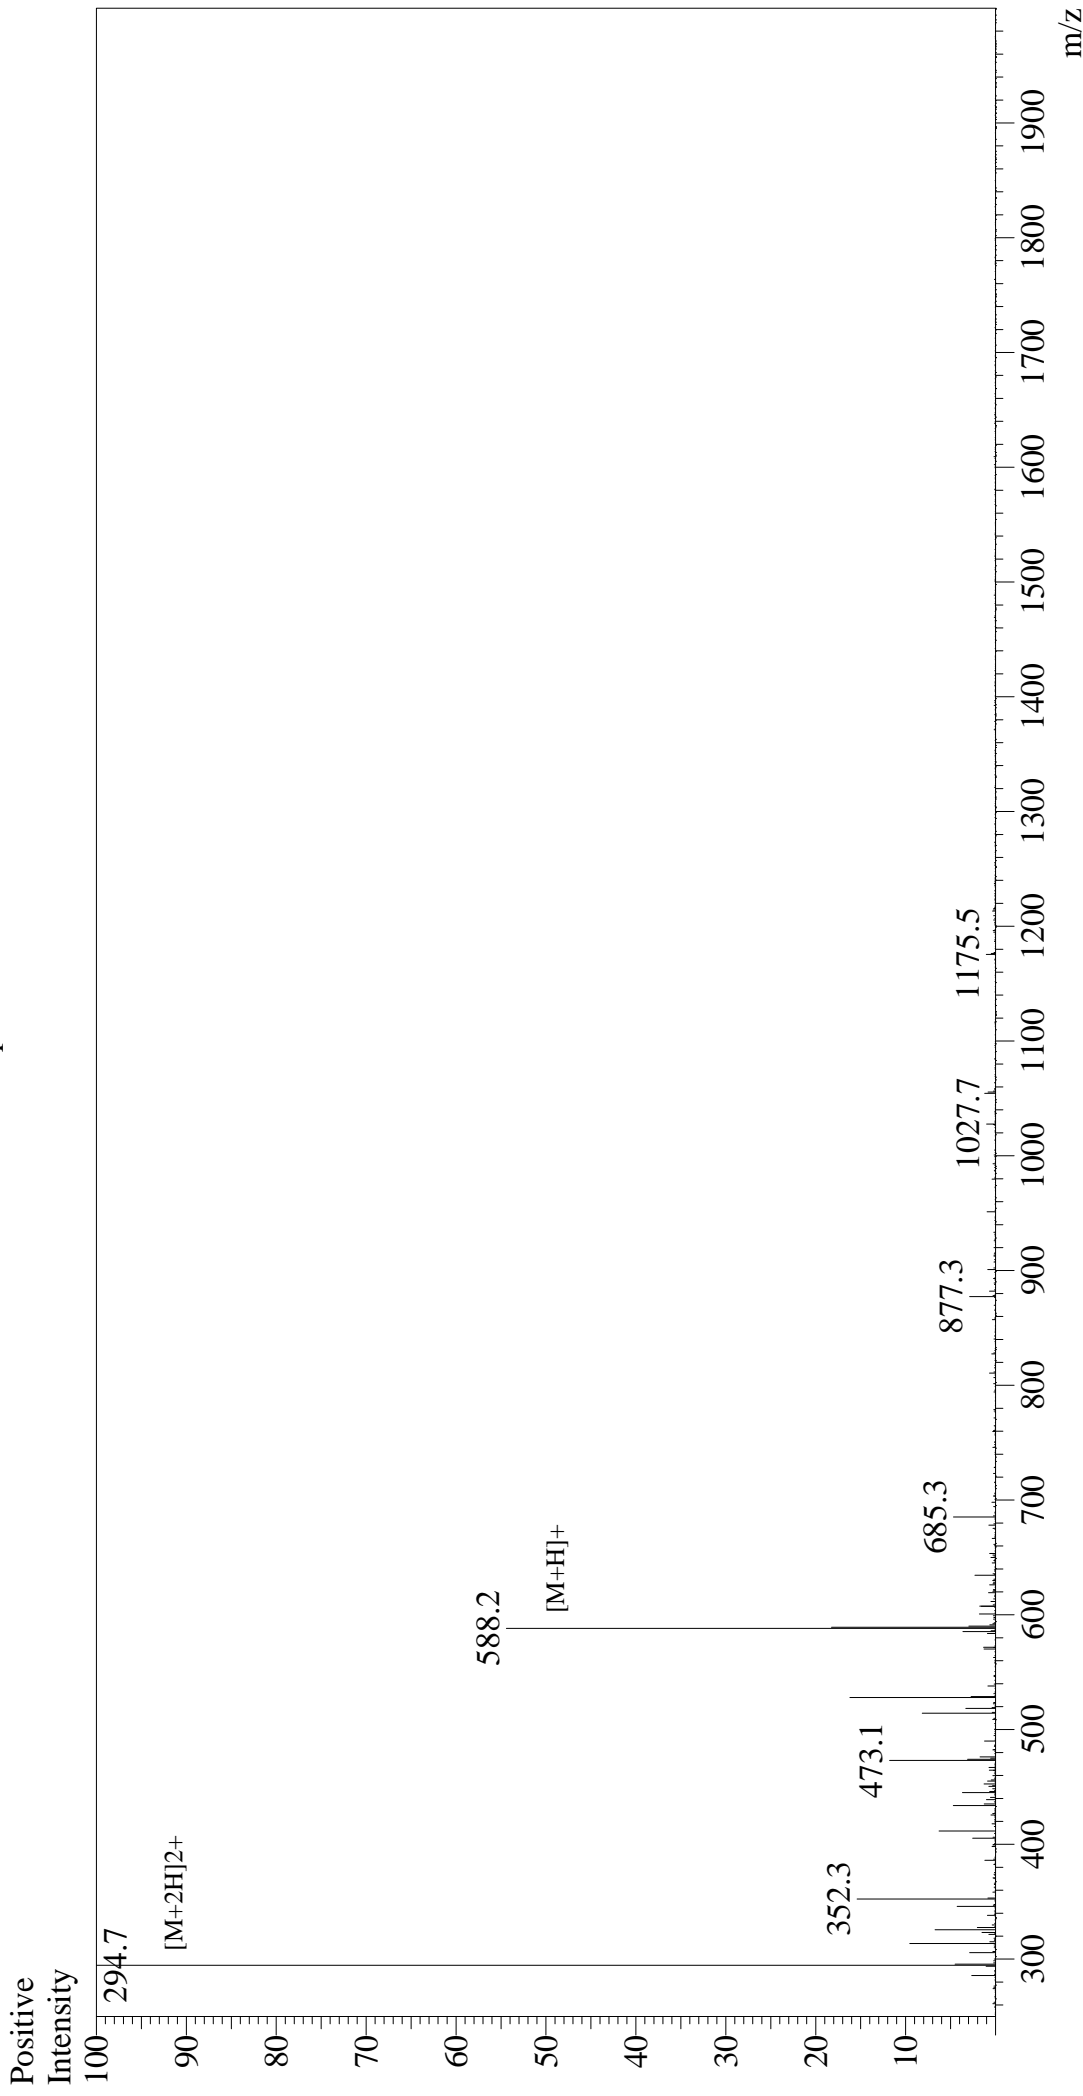

Sample Information

Month-Day Processed :	10/21/20	Equipment :	GK11010007
Time Processed :	19:13:36	Interface Bias :	+4.5 kV
Injection Volume :	0.3	Drying Gas Flow :	5 L/min
Sample Name :	GRGDSP	T.Flow :	0.2 ml/min
Cat. No. :	RP20255	B.conc :	50% H2O/50% MeOH
Lot. No. :	E6296020J		
Theoretical MW :	587.59		
Observed MW :	587.4		

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200