

Sample Name :  $\beta$ -Amyloid (1-15)  
 Cat. No. : RP20141  
 Lot. No. : PE3421612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima<sup>TM</sup> C18 4.6 x 250 mm

Chromatogram

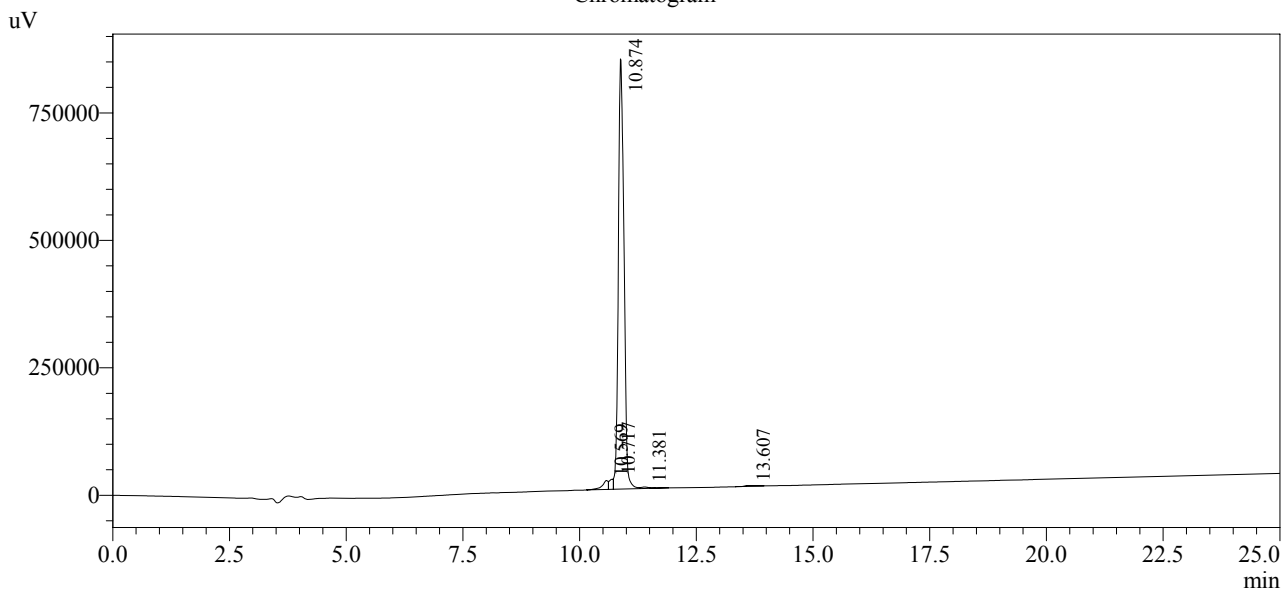

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.569	158309	17570	2.140
2	10.717	120591	19824	1.630
3	10.874	7055225	844004	95.359
4	11.381	40721	2924	0.550
5	13.607	23783	1650	0.321
Total		7398629	885972	100.000