

Sample Name :HIF-1 alpha (556-574)
 Cat No :RP20479
 Lot No :E0645321A
 Time Processed :18:42:57
 Month-Day-Year Processed :01/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

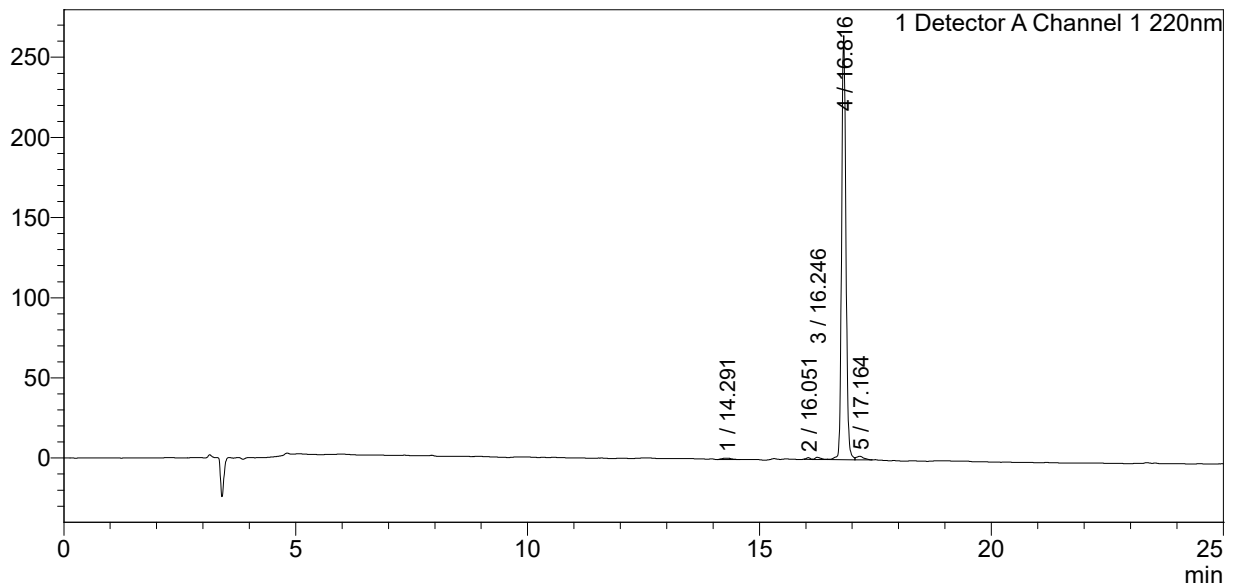

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.291	12144	862	0.692
2	16.051	5804	1080	0.331
3	16.246	11000	1336	0.627
4	16.816	1702597	264571	96.979
5	17.164	24089	2169	1.372
Total		1755634	270017	100.000