

Sample Name :Flagelin22  
 Cat No. :RP19986  
 Lot No. :E7131921C  
 Time Processed :11:26:28 AM  
 Month-Day-Year Processed :04/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
25.00	Pumps	B.Conc	50
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

<Chromatogram>

mV

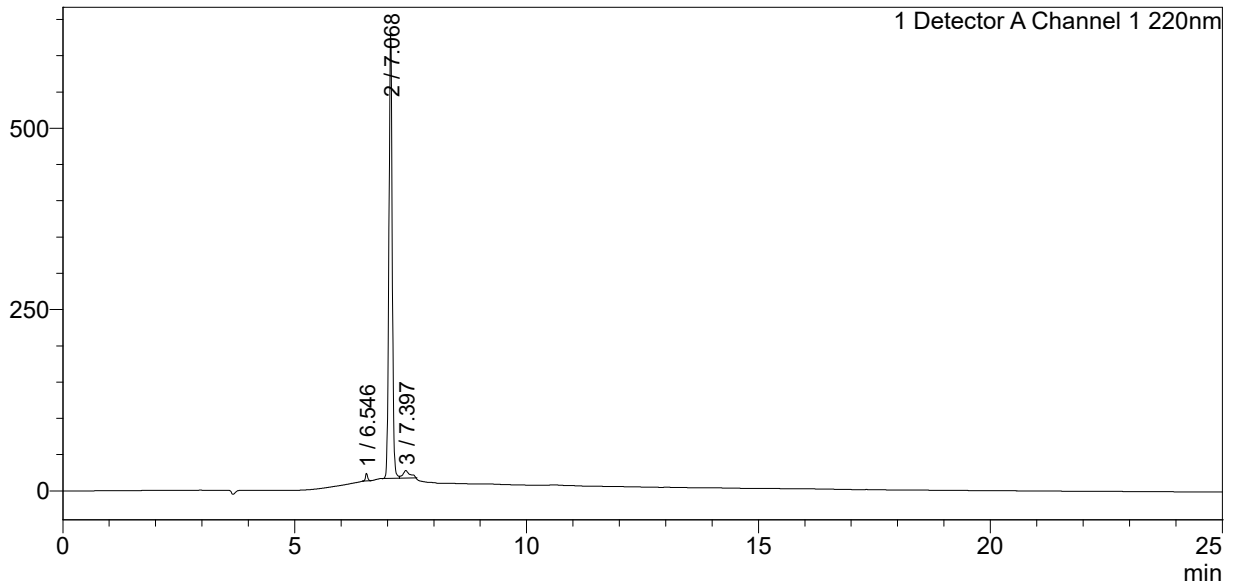

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.546	34115	10411	1.072
2	7.068	3032847	613868	95.304
3	7.397	115335	10516	3.624
Total		3182297	634795	100.000