

Sample Name :c-Myc Peptide  
 Cat. No. : RP11731  
 Lot. No. : PE1921903  
 Time Processed : 14:09:11  
 Month-Day-Year Processed : 03/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
32.00	Pumps	Pump B Conc.	95	
32.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

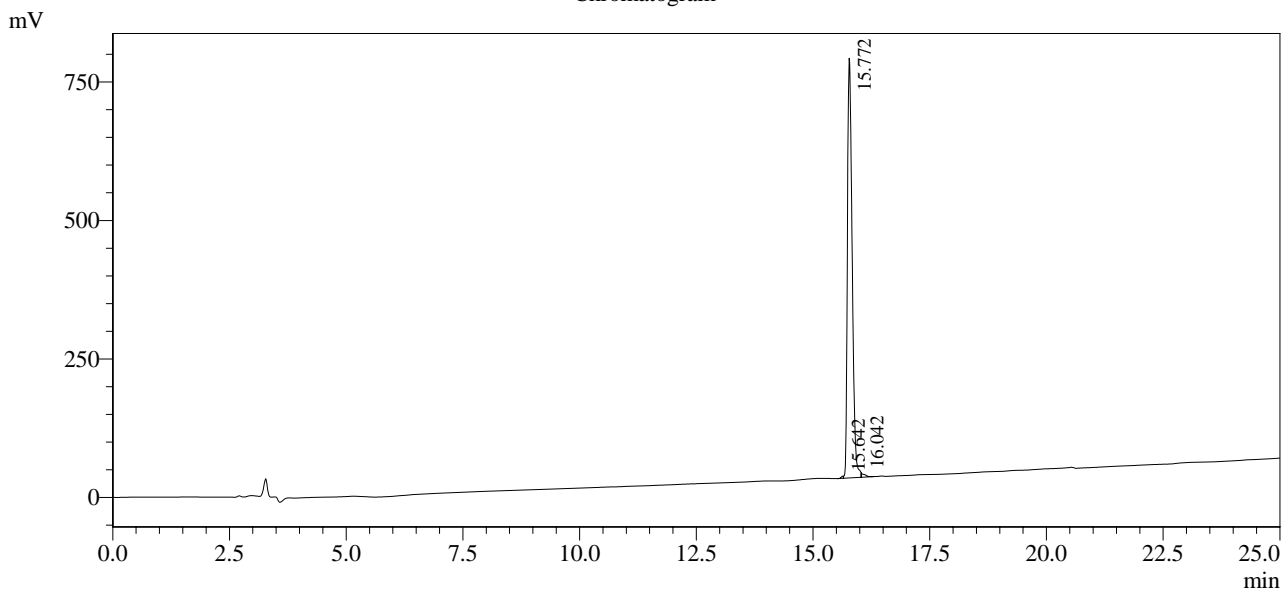

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.642	13162	4010	0.244
2	15.772	5341753	757577	99.091
3	16.042	35829	7031	0.665
Total		5390745	768618	100.000