

Sample Name: Somatostatin
 Cat No: RP10226
 Lot No : E1173420K
 Time Processed : 8:44:45
 Month-Day-Year Processed : 11/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

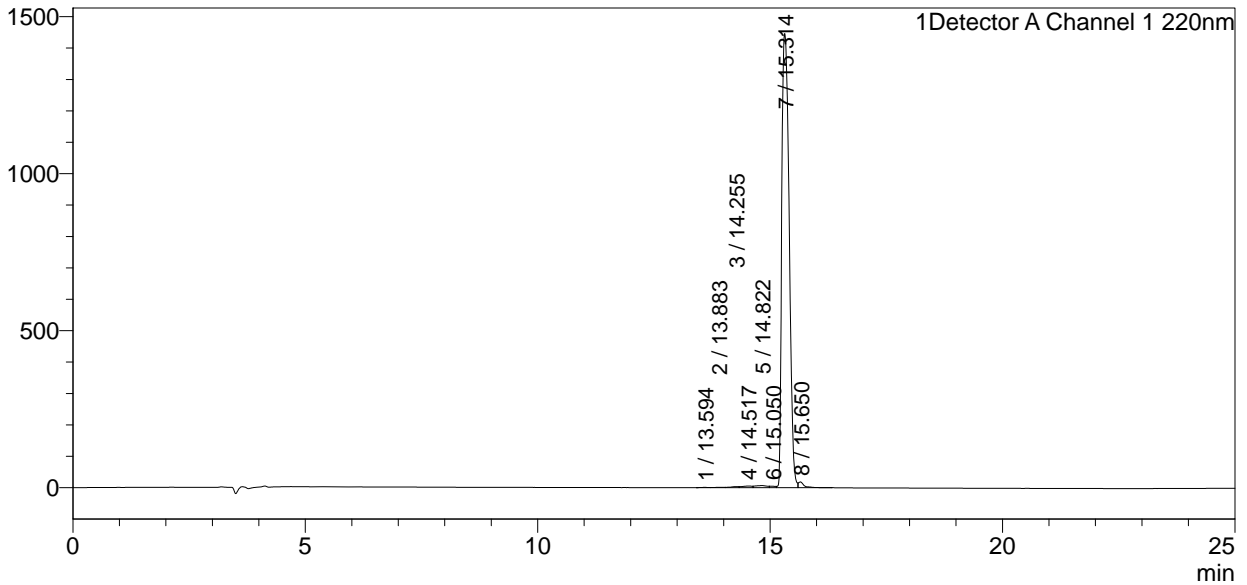

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.594	7029	776	0.043
2	13.883	13739	937	0.084
3	14.255	40937	3501	0.251
4	14.517	78255	4938	0.479
5	14.822	118025	6587	0.723
6	15.050	39410	4608	0.241
7	15.314	15880845	1445596	97.227
8	15.650	155533	18325	0.952
Total		16333773	1485268	100.000