

Sample Name :Corticotropin Releasing Factor, human, rat  
 Cat No :RP10982  
 Lot No :E5907520K  
 Time Processed :7:54:41  
 Month-Day-Year Processed :11/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

### <Chromatogram>

mV

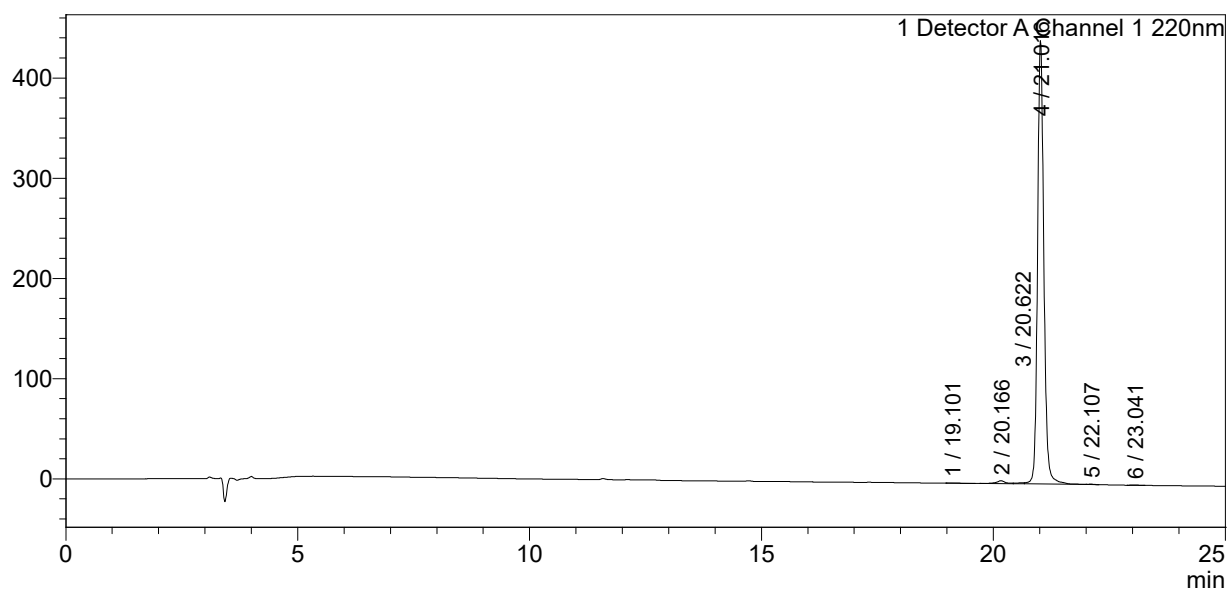

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.101	3983	252	0.094
2	20.166	41759	2972	0.985
3	20.622	12754	1193	0.301
4	21.016	4176162	442525	98.483
5	22.107	2811	356	0.066
6	23.041	3043	256	0.072
Total		4240511	447554	100.000