

Sample Name :β-Amyloid (25-35)

Cat. No. : RP10008

Lot. No. : PE8761904

Time Processed : 21:31:42

Month-Day-Year Processed :04/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:SS-CM-0286

### Chromatogram

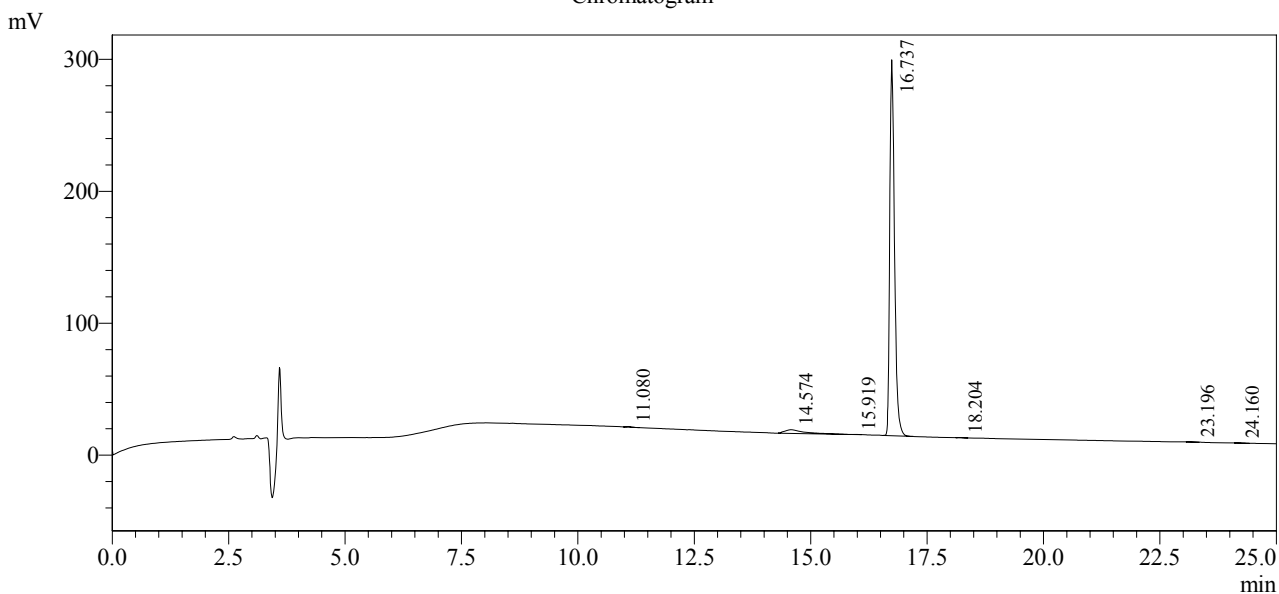

### Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.080	2932	442	0.138
2	14.574	83625	2805	3.937
3	15.919	1018	129	0.048
4	16.737	2032040	284872	95.656
5	18.204	1296	191	0.061
6	23.196	2154	314	0.101
7	24.160	1265	99	0.060
Total		2124329	288852	100.000