

Sample Name :Endomorphin-1
 Cat No.: RP10925
 Lot No.: E6240220H
 Time Processed :7:02:42
 Month-Day-Year Processed :08/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

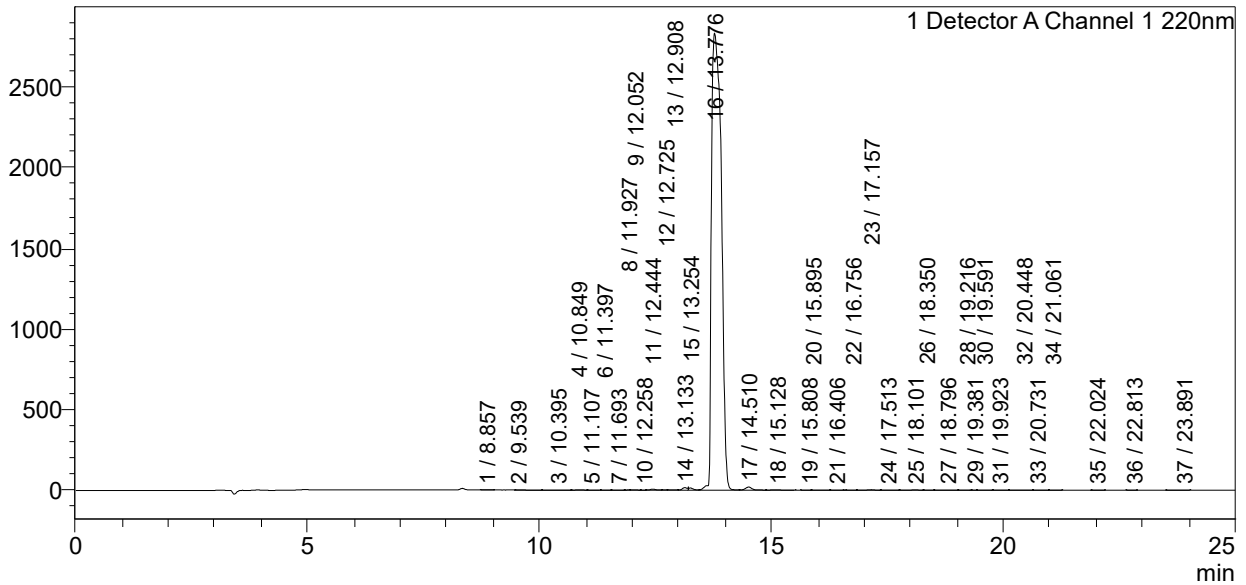

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.857	1115	187	0.003
2	9.539	4969	192	0.012
3	10.395	5037	305	0.012
4	10.849	13963	1603	0.033
5	11.107	3375	332	0.008
6	11.397	1549	181	0.004
7	11.693	2734	238	0.006
8	11.927	3907	630	0.009
9	12.052	10495	1327	0.025
10	12.258	3013	492	0.007
11	12.444	51396	6063	0.122
12	12.725	7640	1023	0.018
13	12.908	19422	1653	0.046
14	13.133	108946	15545	0.258
15	13.254	96810	12959	0.229

Peak#	Ret. Time	Area	Height	Area%
16	13.776	41588991	2836476	98.365
17	14.510	191319	19159	0.453
18	15.128	16629	895	0.039
19	15.808	2852	340	0.007
20	15.895	4262	351	0.010
21	16.406	2342	260	0.006
22	16.756	4123	411	0.010
23	17.157	30866	3021	0.073
24	17.513	8652	567	0.020
25	18.101	24100	1731	0.057
26	18.350	11309	1005	0.027
27	18.796	18336	1165	0.043
28	19.216	3151	297	0.007
29	19.381	3080	331	0.007
30	19.591	5899	432	0.014
31	19.923	7133	402	0.017
32	20.448	10414	496	0.025
33	20.731	5134	370	0.012
34	21.061	2613	194	0.006
35	22.024	1282	108	0.003
36	22.813	1631	165	0.004
37	23.891	1664	97	0.004
Total		42280154	2911003	100.000