

Sample Name :YRGDS Fibronectin Fragment
 Cat. No. : RP20476
 Lot. No. : PE9291903
 Time Processed : 10:14:31
 Month-Day-Year Processed : 03/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 27.00 | Pumps | Pump B Conc. | 95 | |
| 27.01 | Pumps | Pump B Conc. | 5 | |
| 35.00 | Pumps | Pump B Conc. | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

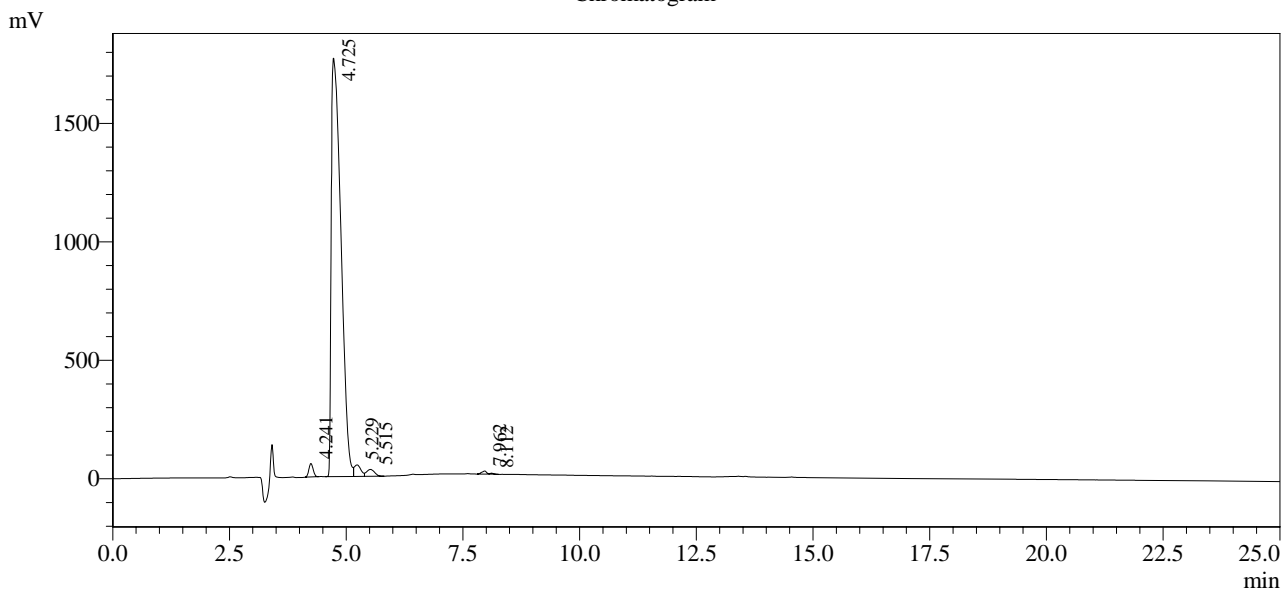

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|----------|---------|---------|
| 1 | 4.241 | 363017 | 56858 | 1.355 |
| 2 | 4.725 | 25497509 | 1765696 | 95.162 |
| 3 | 5.229 | 476162 | 48583 | 1.777 |
| 4 | 5.515 | 344390 | 29123 | 1.285 |
| 5 | 7.962 | 93940 | 13140 | 0.351 |
| 6 | 8.112 | 18767 | 4422 | 0.070 |
| Total | | 26793785 | 1917821 | 100.000 |