

Sample Name :Men 10376  
Cat. No. : RP10468  
Lot. No. : E4802119I  
Time Processed :14:24:22  
Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

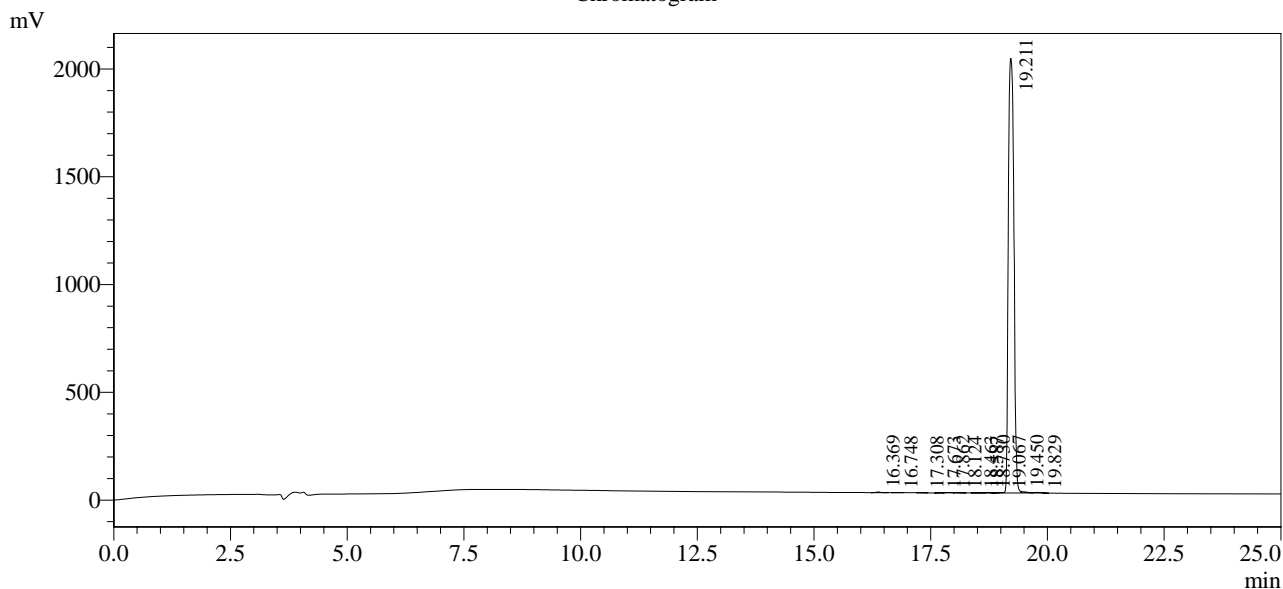

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.369	21054	3001	0.125
2	16.748	3036	448	0.018
3	17.308	3686	564	0.022
4	17.673	2048	430	0.012
5	17.862	12436	1869	0.074
6	18.124	9248	968	0.055
7	18.463	3938	748	0.023
8	18.587	7598	1351	0.045
9	18.730	12347	1979	0.073
10	19.067	16702	2730	0.099
11	19.211	16626073	2017016	98.934
12	19.450	49680	5857	0.296
13	19.829	37363	3248	0.222
Total		16805209	2040208	100.000