

Sample Name : $\delta$ -Sleep Inducing Peptide  
 Cat. No. : RP10580  
 Lot. No. : E474419I  
 Time Processed : 7:46:24  
 Month-Day-Year Processed : 09/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

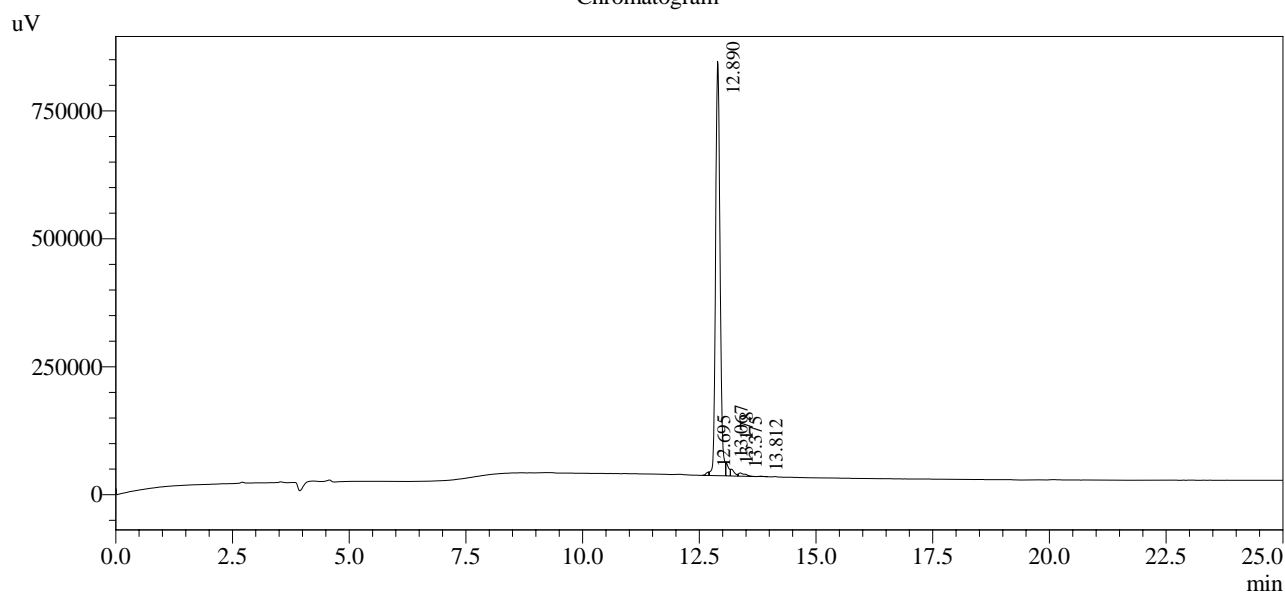

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.695	29186	6863	0.512
2	12.890	5419899	809717	95.128
3	13.067	108012	26495	1.896
4	13.178	73350	13269	1.287
5	13.375	62565	6372	1.098
6	13.812	4488	713	0.079
Total		5697499	863429	100.000