

Sample Name : OVA G4 peptide  
 Cat. No. : RP20398  
 Lot. No. : E3495619K  
 Time Processed : 5:23:37  
 Month-Day-Year Processed : 11/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

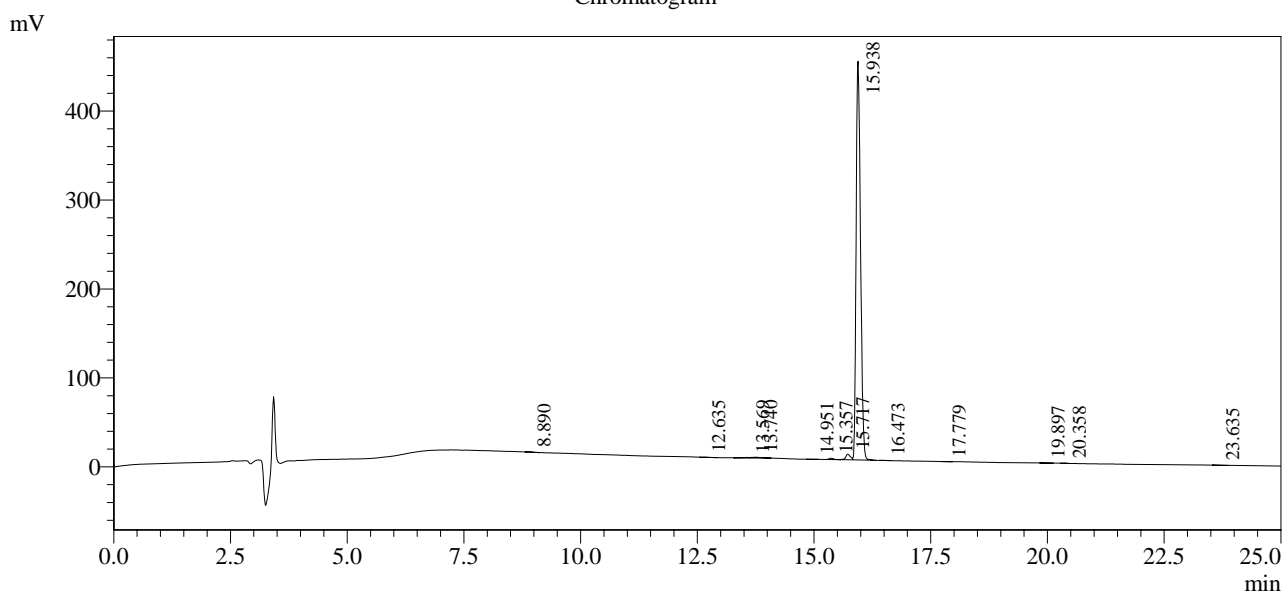

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.890	3116	451	0.103
2	12.635	1690	168	0.056
3	13.569	6658	598	0.219
4	13.740	14015	947	0.461
5	14.951	1654	256	0.054
6	15.357	10416	1529	0.343
7	15.717	43802	6324	1.442
8	15.938	2947157	448255	97.012
9	16.473	1732	302	0.057
10	17.779	1147	116	0.038
11	19.897	1250	161	0.041
12	20.358	2773	467	0.091
13	23.635	2512	318	0.083
Total		3037921	459892	100.000