


Mass Spectrum

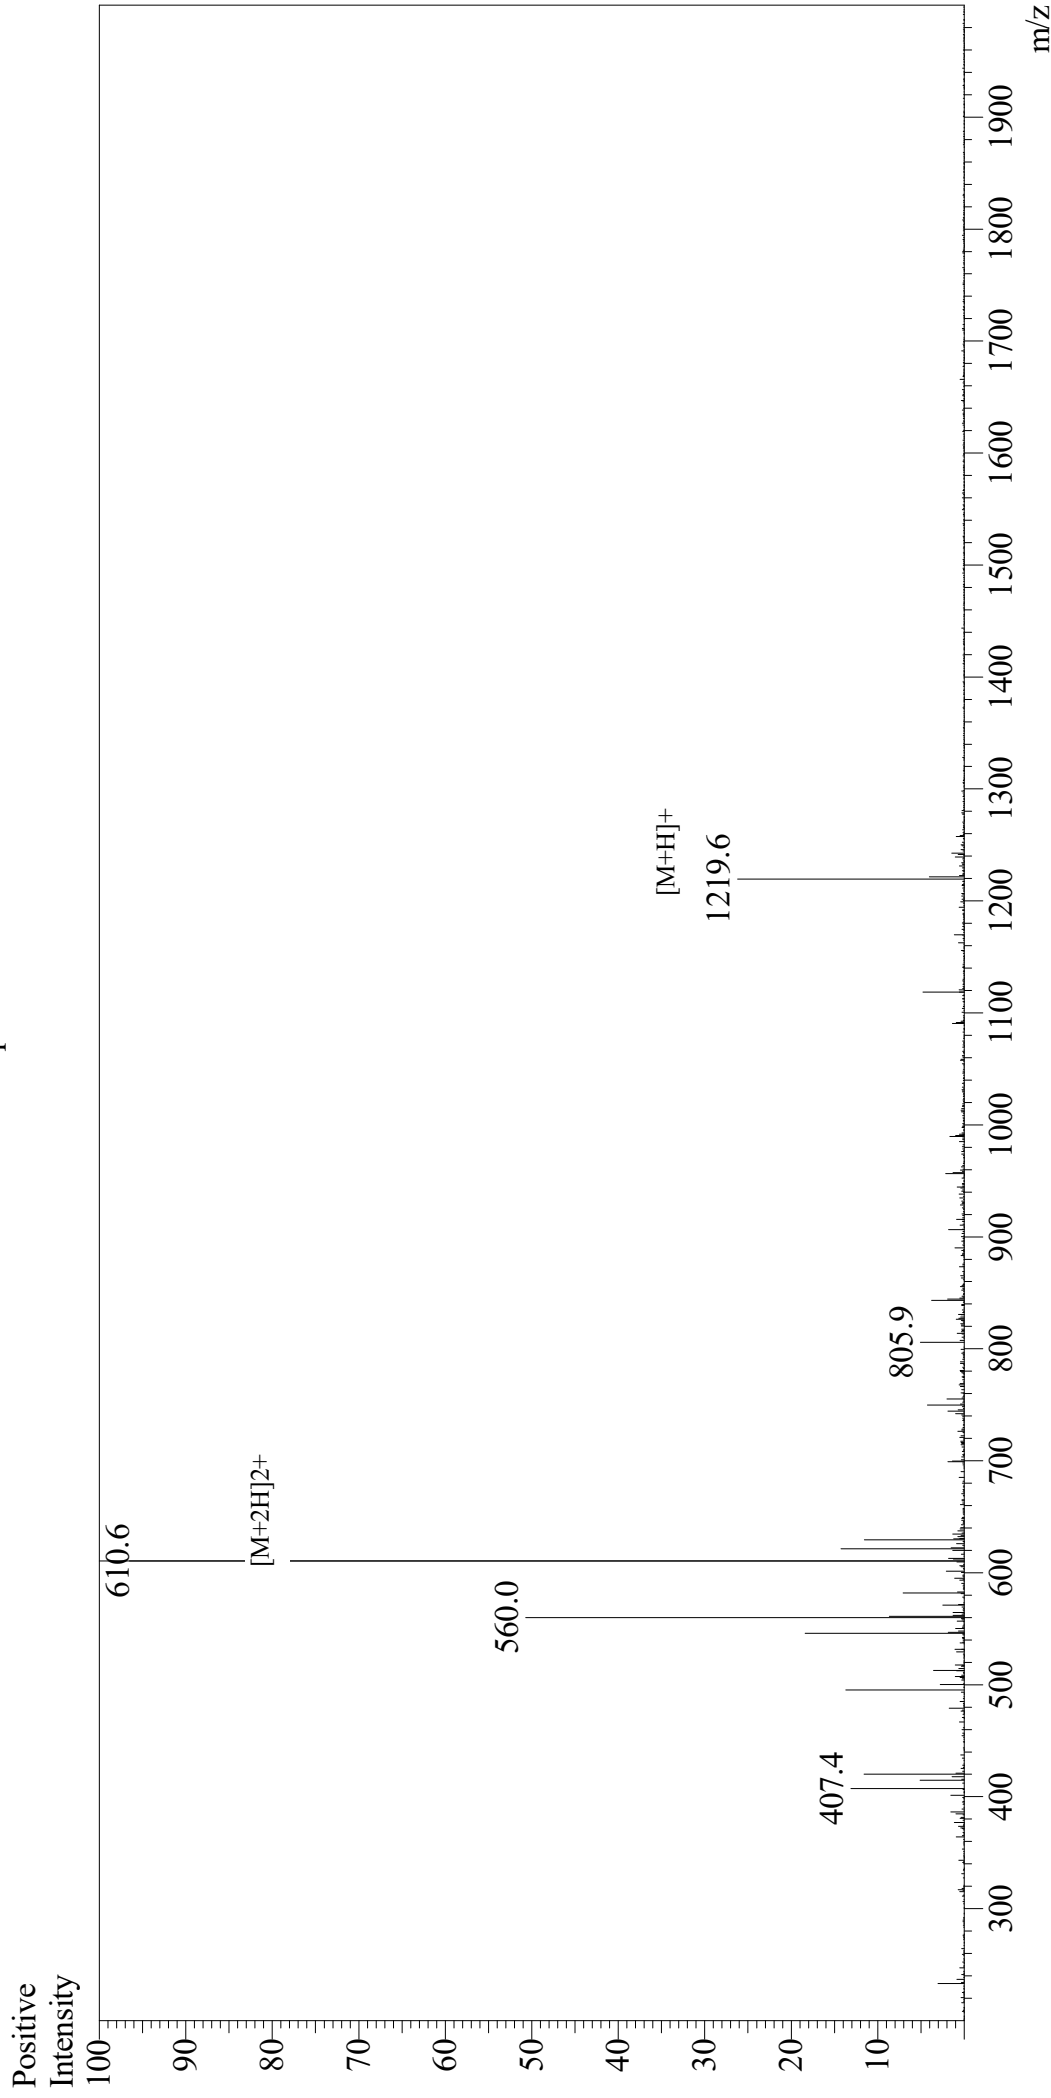

Sample Information

User : Gary
Month-Day Processed : 09/20/19
Time Processed : 09:53:23 AM
Injection Volume : 0.4
Sample Name : GroES mobile loop
Cat No. : RP20179
Lot No. : E4830319I
Theoretical MW : 1219.40
Observed MW : 1219.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH