

Sample Name :CEF27, Epstein-Barr Virus BRLF-1 lytic (148-156)
Cat No. :RP20397
Lot No. :E4950919I
Time Processed :14:47:05
Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment:ZJ17010507

<Chromatogram>

mV

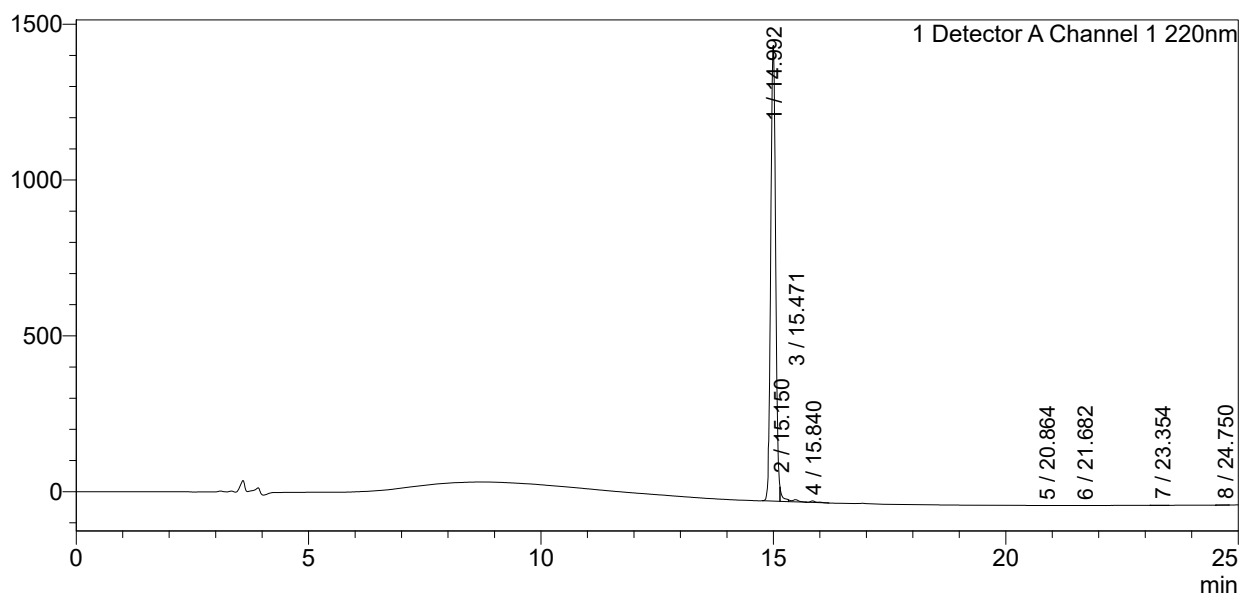

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.992	10764111	1461542	97.583
2	15.150	143682	37146	1.303
3	15.471	74172	7371	0.672
4	15.840	43900	4928	0.398
5	20.864	1559	147	0.014
6	21.682	1148	118	0.010
7	23.354	1076	122	0.010
8	24.750	1056	69	0.010
Total		11030703	1511443	100.000