

Sample Name :Angiotensin II (3-8), human
 Cat No. : RP11253
 Lot No. : E6360821H
 Time Processed : 23:31:44
 Month-Day-Year Processed : 08/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

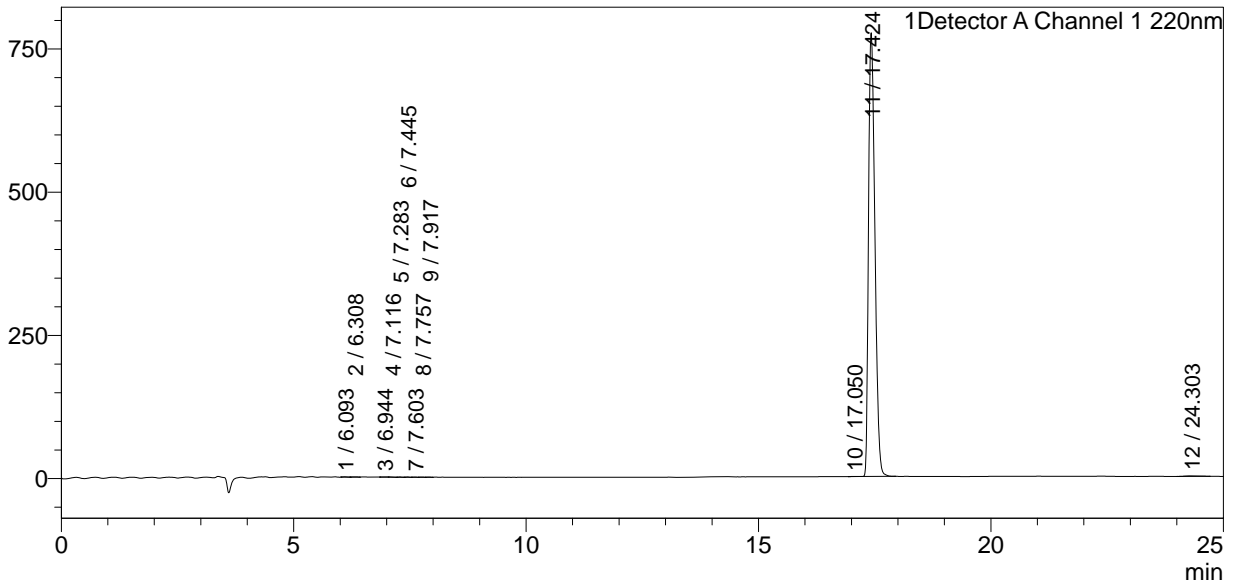

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.093	3374	550	0.045
2	6.308	2408	356	0.032
3	6.944	1611	325	0.022
4	7.116	2034	385	0.027
5	7.283	2090	427	0.028
6	7.445	2055	447	0.028
7	7.603	1846	393	0.025
8	7.757	1660	353	0.022
9	7.917	1307	273	0.018
10	17.050	3454	225	0.046
11	17.424	7398624	770180	99.479
12	24.303	16943	859	0.228
Total		7437407	774772	100.000