

Sample Name: Oxytocin
 Cat No. : RP10407
 Lot No. : E2084720E
 Time Processed: 7:54:38
 Month-Day-Year Processed :05/31/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:ZJ19010014

<Chromatogram>

mV

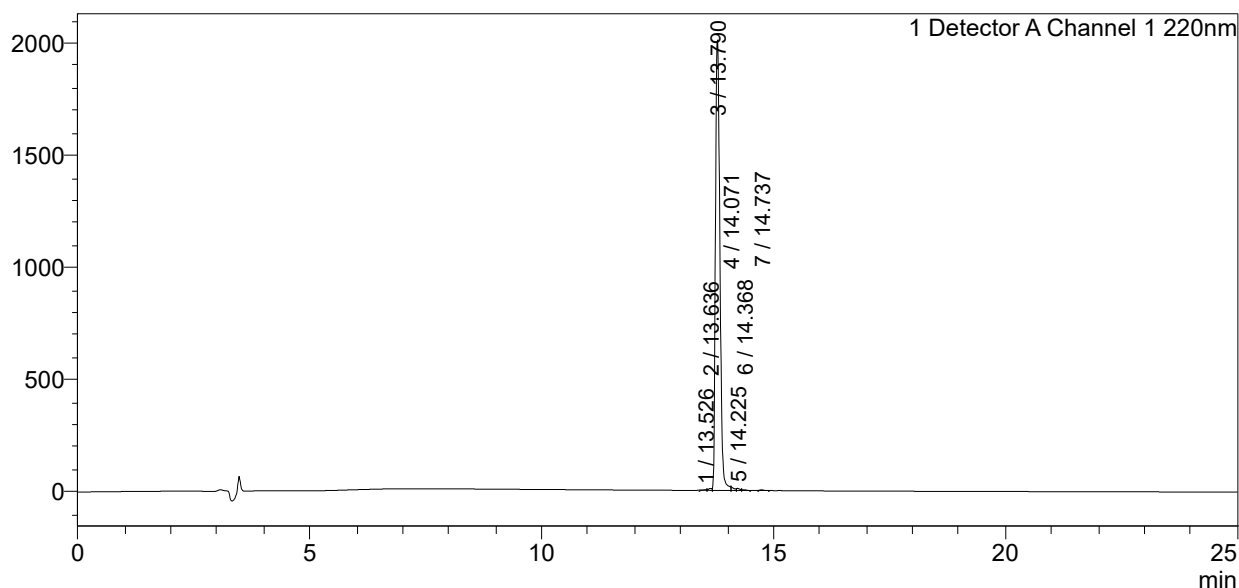

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.526	7122	1690	0.052
2	13.636	40648	8254	0.298
3	13.790	13415464	2007747	98.497
4	14.071	70017	16547	0.514
5	14.225	57287	9060	0.421
6	14.368	10309	2297	0.076
7	14.737	19343	3322	0.142
Total		13620191	2048915	100.000