


# Mass Spectrum

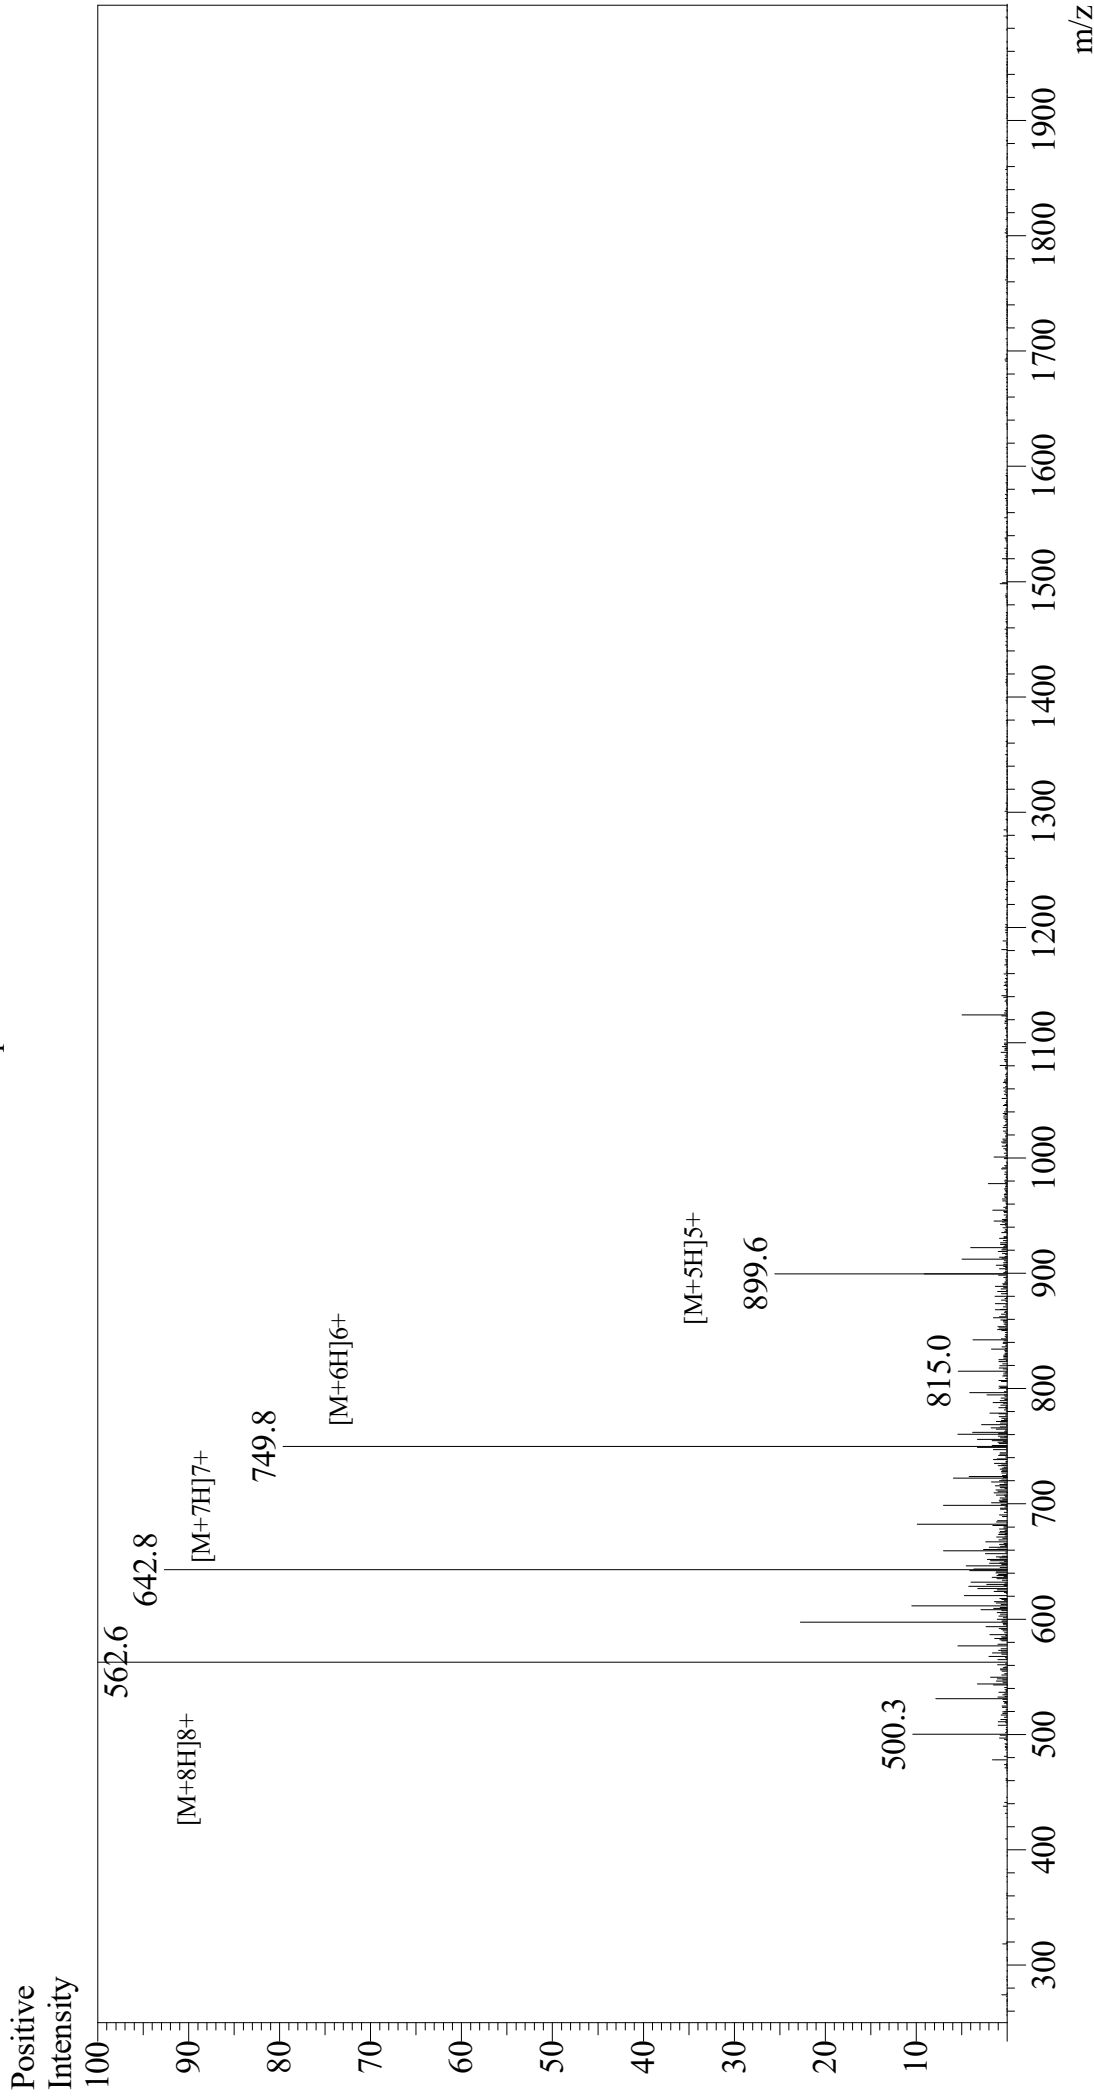

Sample Information  
Month-Day Processed : 04/21/21  
Time Processed : 22:53:33  
Injection Volume : 0.4  
Sample Name : LL - 37, scrambled  
Cat No. : RP20332  
Lot No. : E9430321D  
Theoretical MW : 4493.30  
Observed MW : 4492.8

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH