

Sample Name : Bacterial Sortase Substrate III, Abz/DNP
 Cat. No. :RP20431
 Lot. No. :PE8291807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

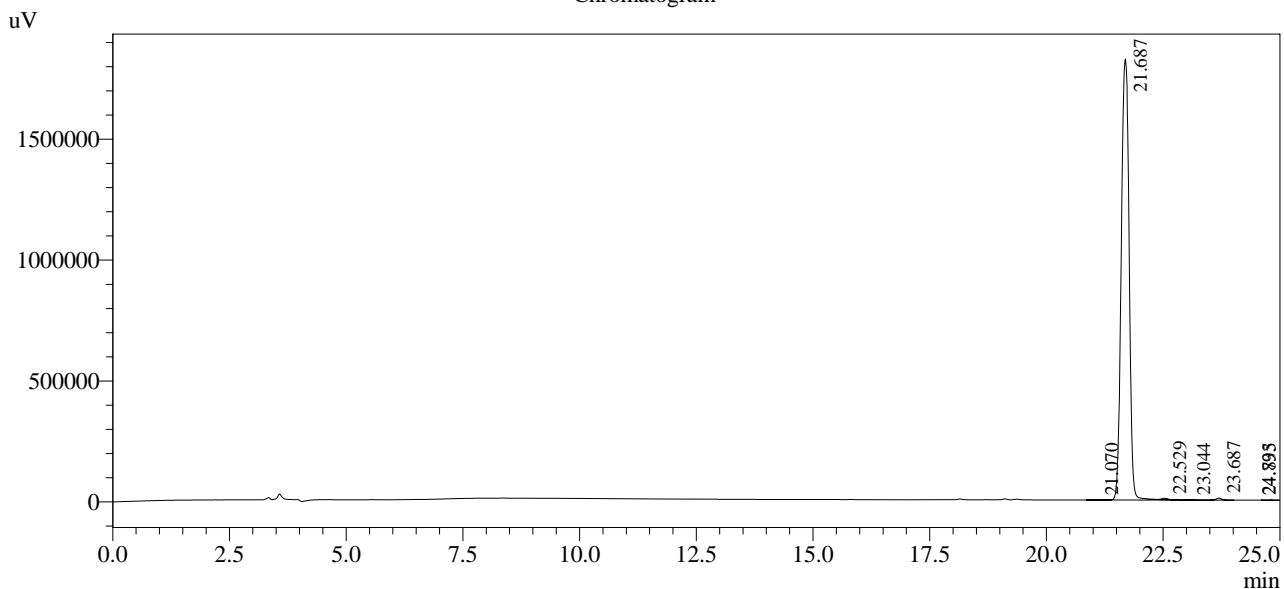

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	21.070	4790	507	0.022
2	21.687	21278216	1824629	99.381
3	22.529	50051	5418	0.234
4	23.044	1979	280	0.009
5	23.687	67028	8111	0.313
6	24.735	3668	485	0.017
7	24.893	5042	642	0.024
Total		21410774	1840071	100.000