


Mass Spectrum

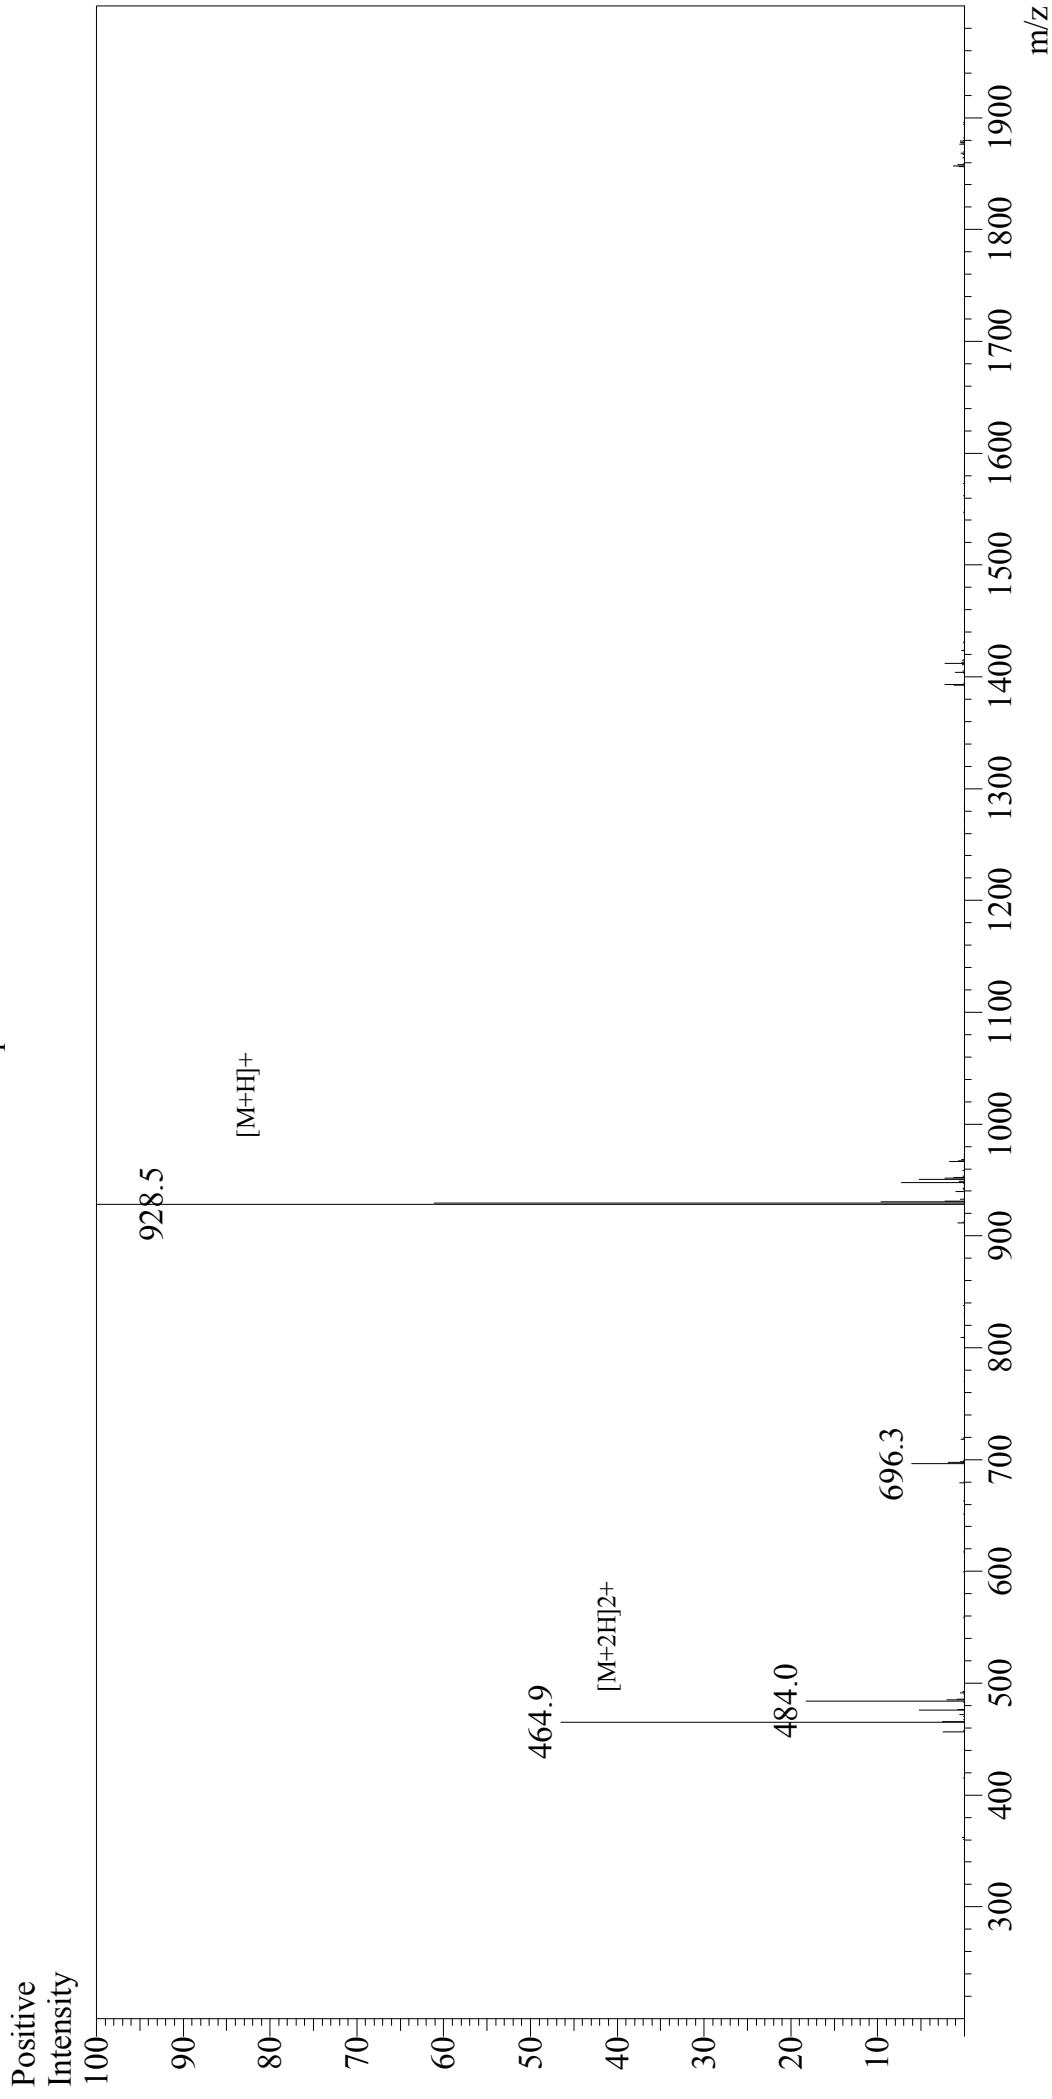

Sample Information

User : Gary
Month-Day Processed : 07/28/18
Time Processed : 20:37:18
Injection Volume : 0.2
Sample Name : Bacterial Sortase Substrate III, Abz/DNIP
Cat No. : RP20431
Lot No. : PE8291807
Theoretical MW : 928.00
Observed MW : 927.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH