

Sample Name :Influenza A NP(366-374) Strain A/PR/8/35  
 Cat No. :RP20267  
 Lot No. :E3425221B  
 Time Processed :23:13:48  
 Month-Day-Year Processed :02/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

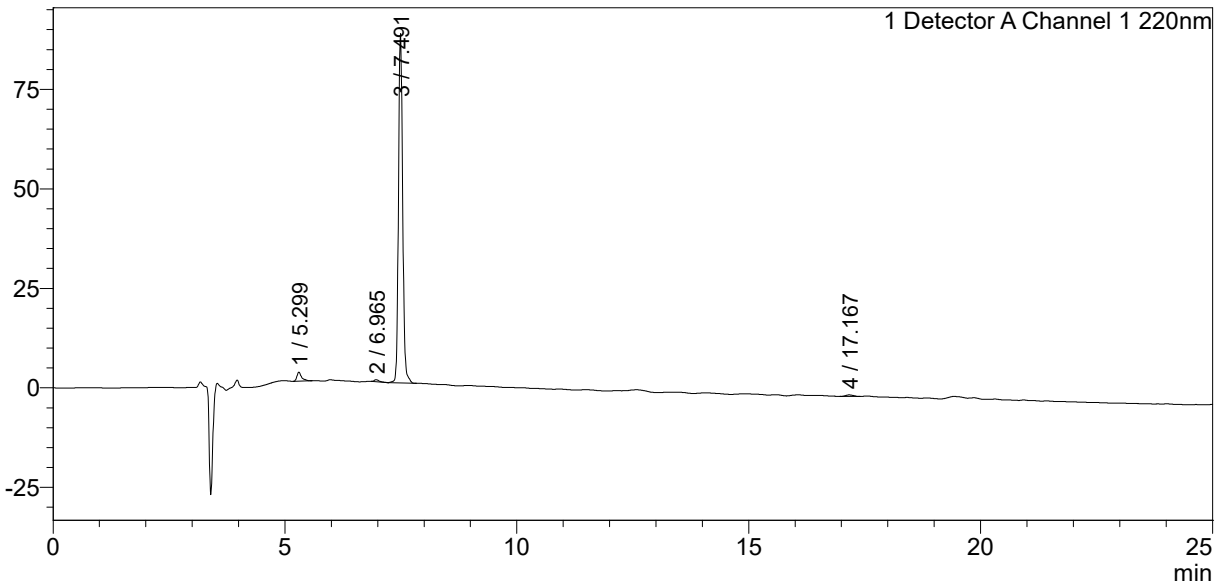

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.299	16257	2265	2.830
2	6.965	3711	521	0.646
3	7.491	549823	86515	95.715
4	17.167	4643	393	0.808
Total		574435	89694	100.000