

Sample Name : Human Papillomavirus (HPV) E7 protein (49 - 57)
Cat. No. : RP20249
Lot. No. : PE8461807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

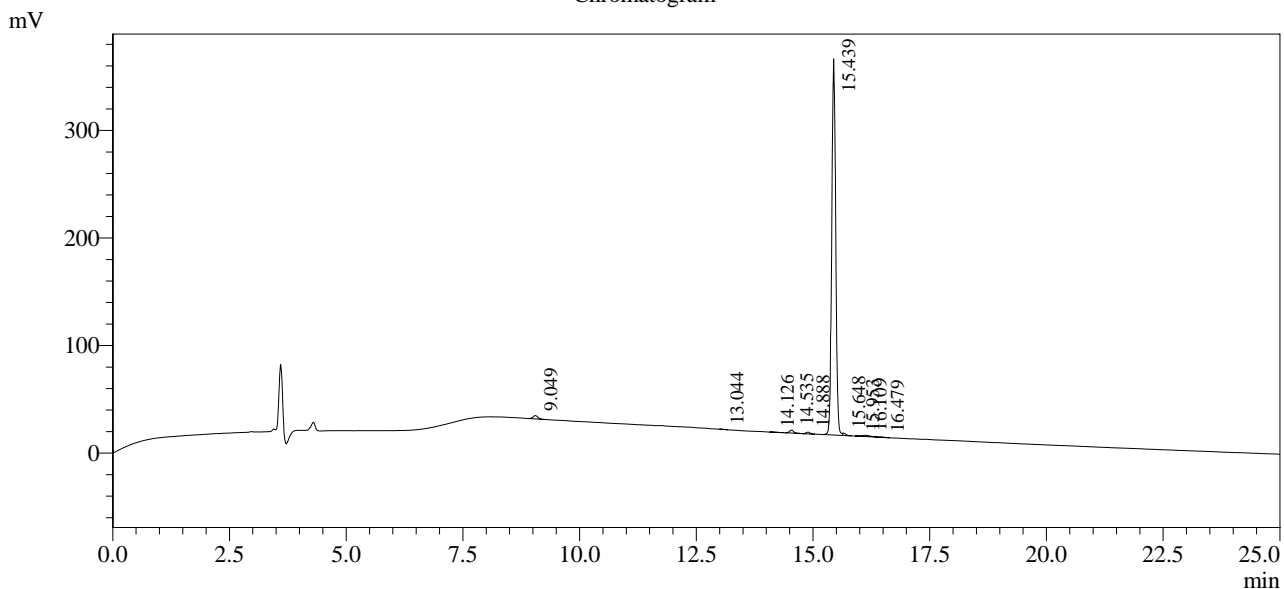

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.049	21685	3101	1.008
2	13.044	1101	237	0.051
3	14.126	1821	218	0.085
4	14.535	18233	2862	0.848
5	14.888	9336	1660	0.434
6	15.439	2073953	349737	96.414
7	15.648	9449	2186	0.439
8	15.953	1213	199	0.056
9	16.109	12836	1044	0.597
10	16.479	1466	300	0.068
Total		2151094	361545	100.000