

Sample Name :C-telopeptide
 Cat. No. : RP10566 Lot. No. : PE0221812
 Time Processed : 15:34:18
 Month-Day-Year Processed : 01/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	15	
40.00	Pumps	Pump B Conc.	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

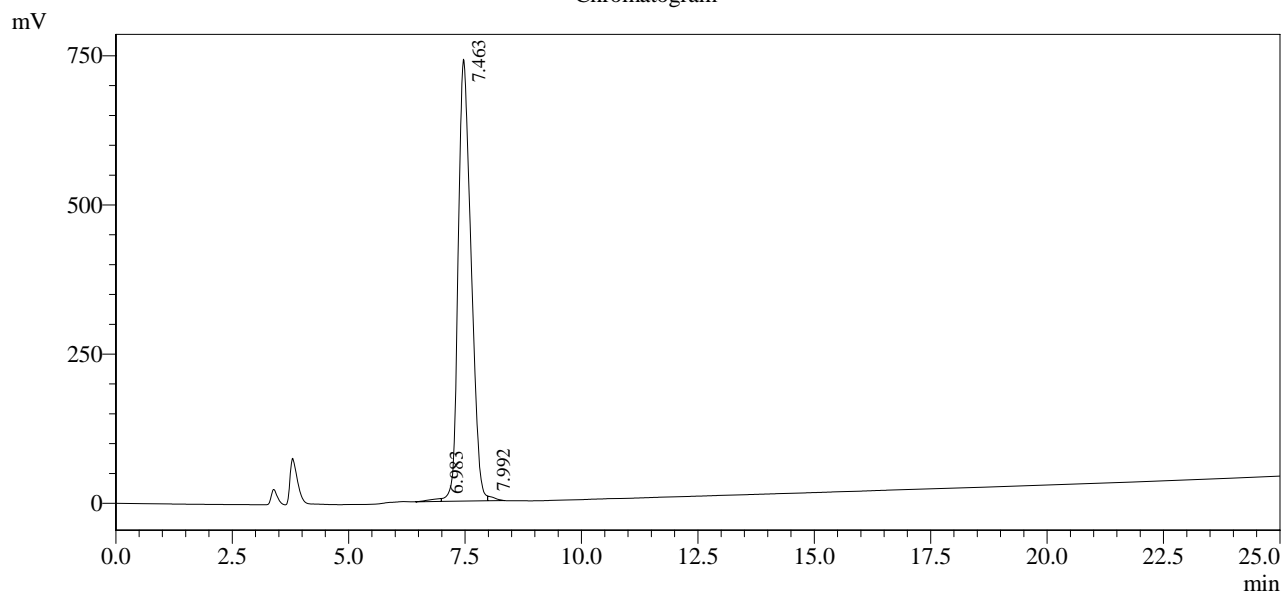

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.983	84950	4806	0.591
2	7.463	14210288	740576	98.871
3	7.992	77303	7763	0.538
Total		14372540	753146	100.000