

Sample Name : β -Amyloid (1-15)
 Cat. No. : RP20141
 Lot. No. : PE751902
 Time Processed : 10:46:30
 Month-Day-Year Processed : 02/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

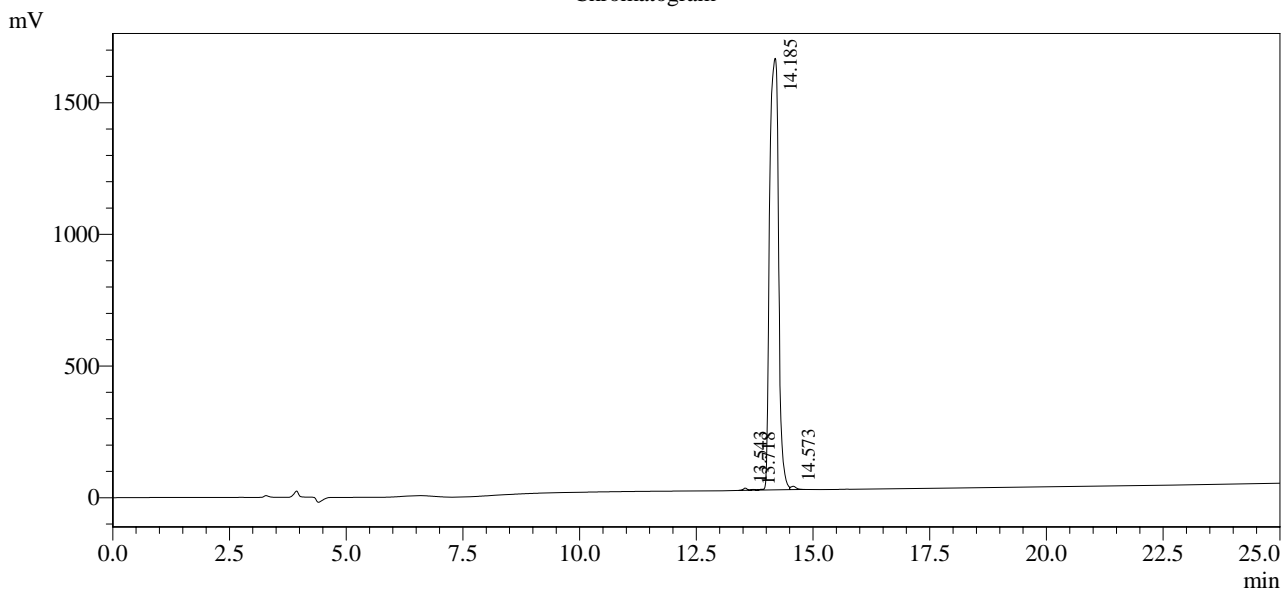

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.543	49913	8387	0.228
2	13.718	16999	2949	0.078
3	14.185	21717979	1639246	99.207
4	14.573	106703	12687	0.487
Total		21891595	1663269	100.000