

Sample Name :Influenza HA (518-526)
 Cat. No. : RP20284
 Lot. No. : E8709621C
 Time Processed :6:44:38 AM
 Month-Day-Year Processed :03/20/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010009

<Chromatogram>

mV

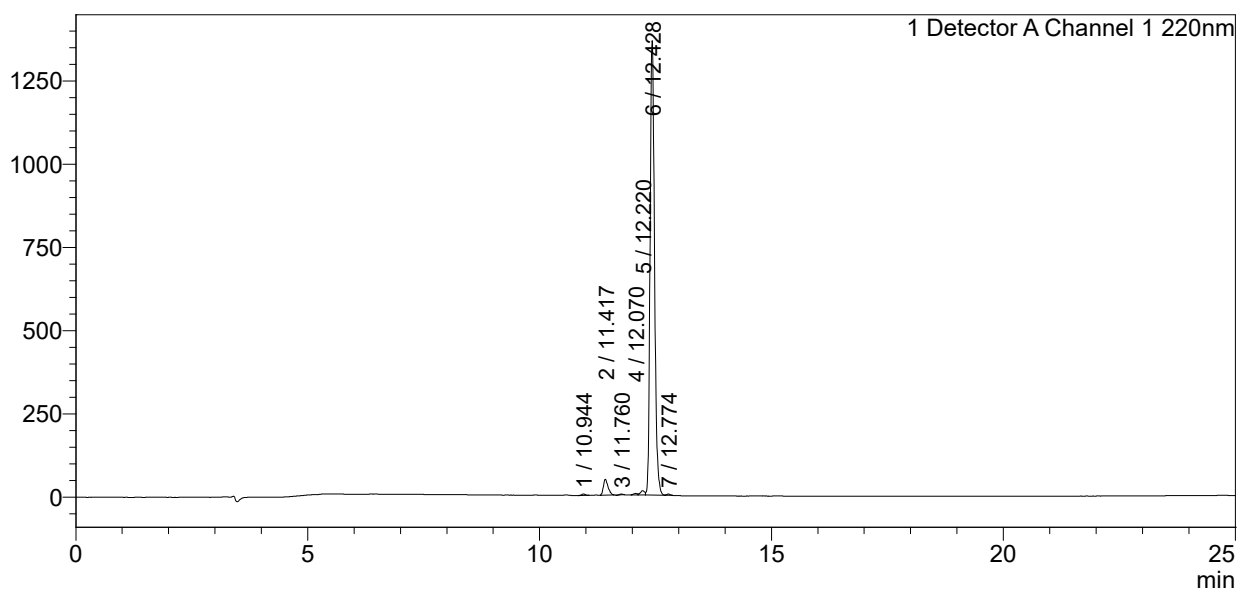

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.944	22274	4048	0.233
2	11.417	327437	47468	3.419
3	11.760	9894	2078	0.103
4	12.070	23619	4177	0.247
5	12.220	78666	12646	0.821
6	12.428	9099757	1365211	95.008
7	12.774	16232	3431	0.169
Total		9577877	1439060	100.000