

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), rat
 Cat No. :RP11195
 Lot No. :E9395021G
 Time Processed : 10:41:48 AM
 Month-Day-Year Processed : 07/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

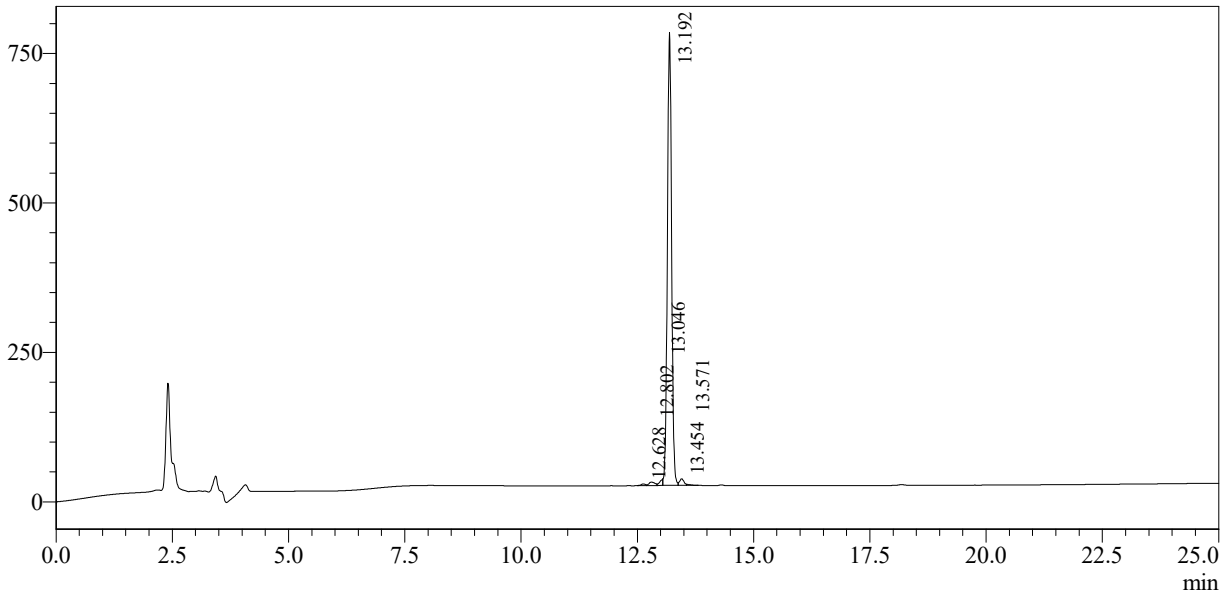

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.628	17203	2765	0.342
2	12.802	50209	5579	0.999
3	13.046	49490	10151	0.985
4	13.192	4826731	757549	96.065
5	13.454	72310	11057	1.439
6	13.571	8490	1597	0.169
Total		5024434	788698	100.000