

Sample Name:Oxytocin
 Cat No :RP10407
 Lot No :E0927821E
 Time Processed :12:21:19 AM
 Month-Day-Year Processed :05/26/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

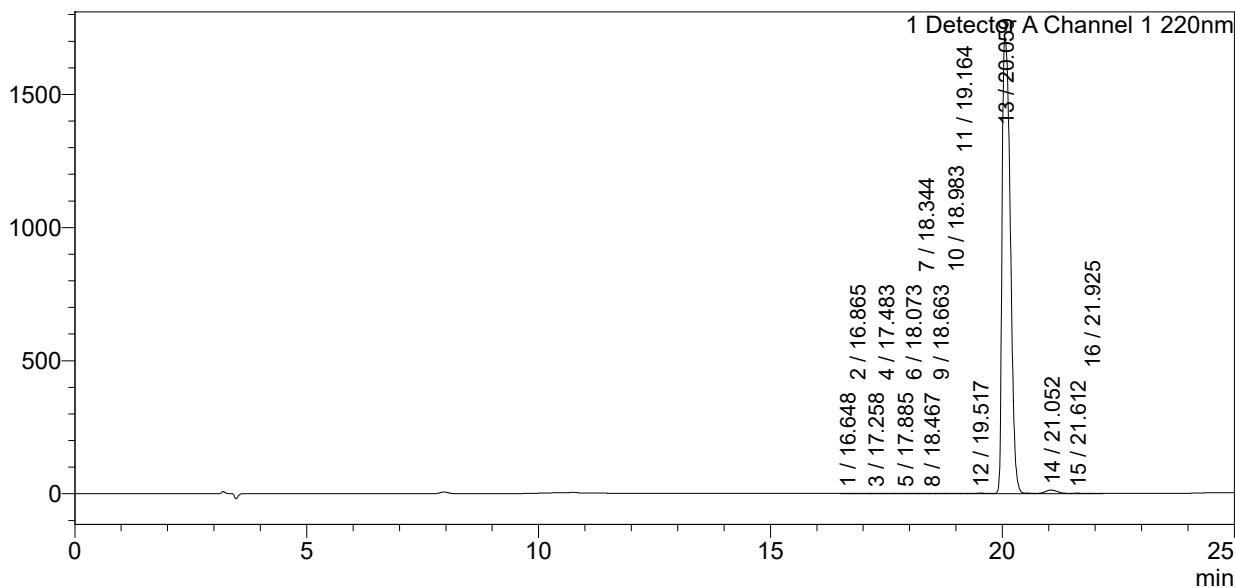

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.648	21100	1655	0.097
2	16.865	38264	1703	0.175
3	17.258	21366	1382	0.098
4	17.483	19017	1269	0.087
5	17.885	22410	1327	0.102
6	18.073	17649	1292	0.081
7	18.344	16662	1323	0.076
8	18.467	10697	1278	0.049
9	18.663	15768	1293	0.072
10	18.983	30472	1792	0.139
11	19.164	12194	1470	0.056
12	19.517	64038	2528	0.293
13	20.059	21206622	1713246	96.995
14	21.052	295272	14387	1.351
15	21.612	47556	2783	0.218

Peak#	Ret. Time	Area	Height	Area%
16	21.925	24450	1598	0.112
Total		21863537	1750325	100.000