


Mass Spectrum

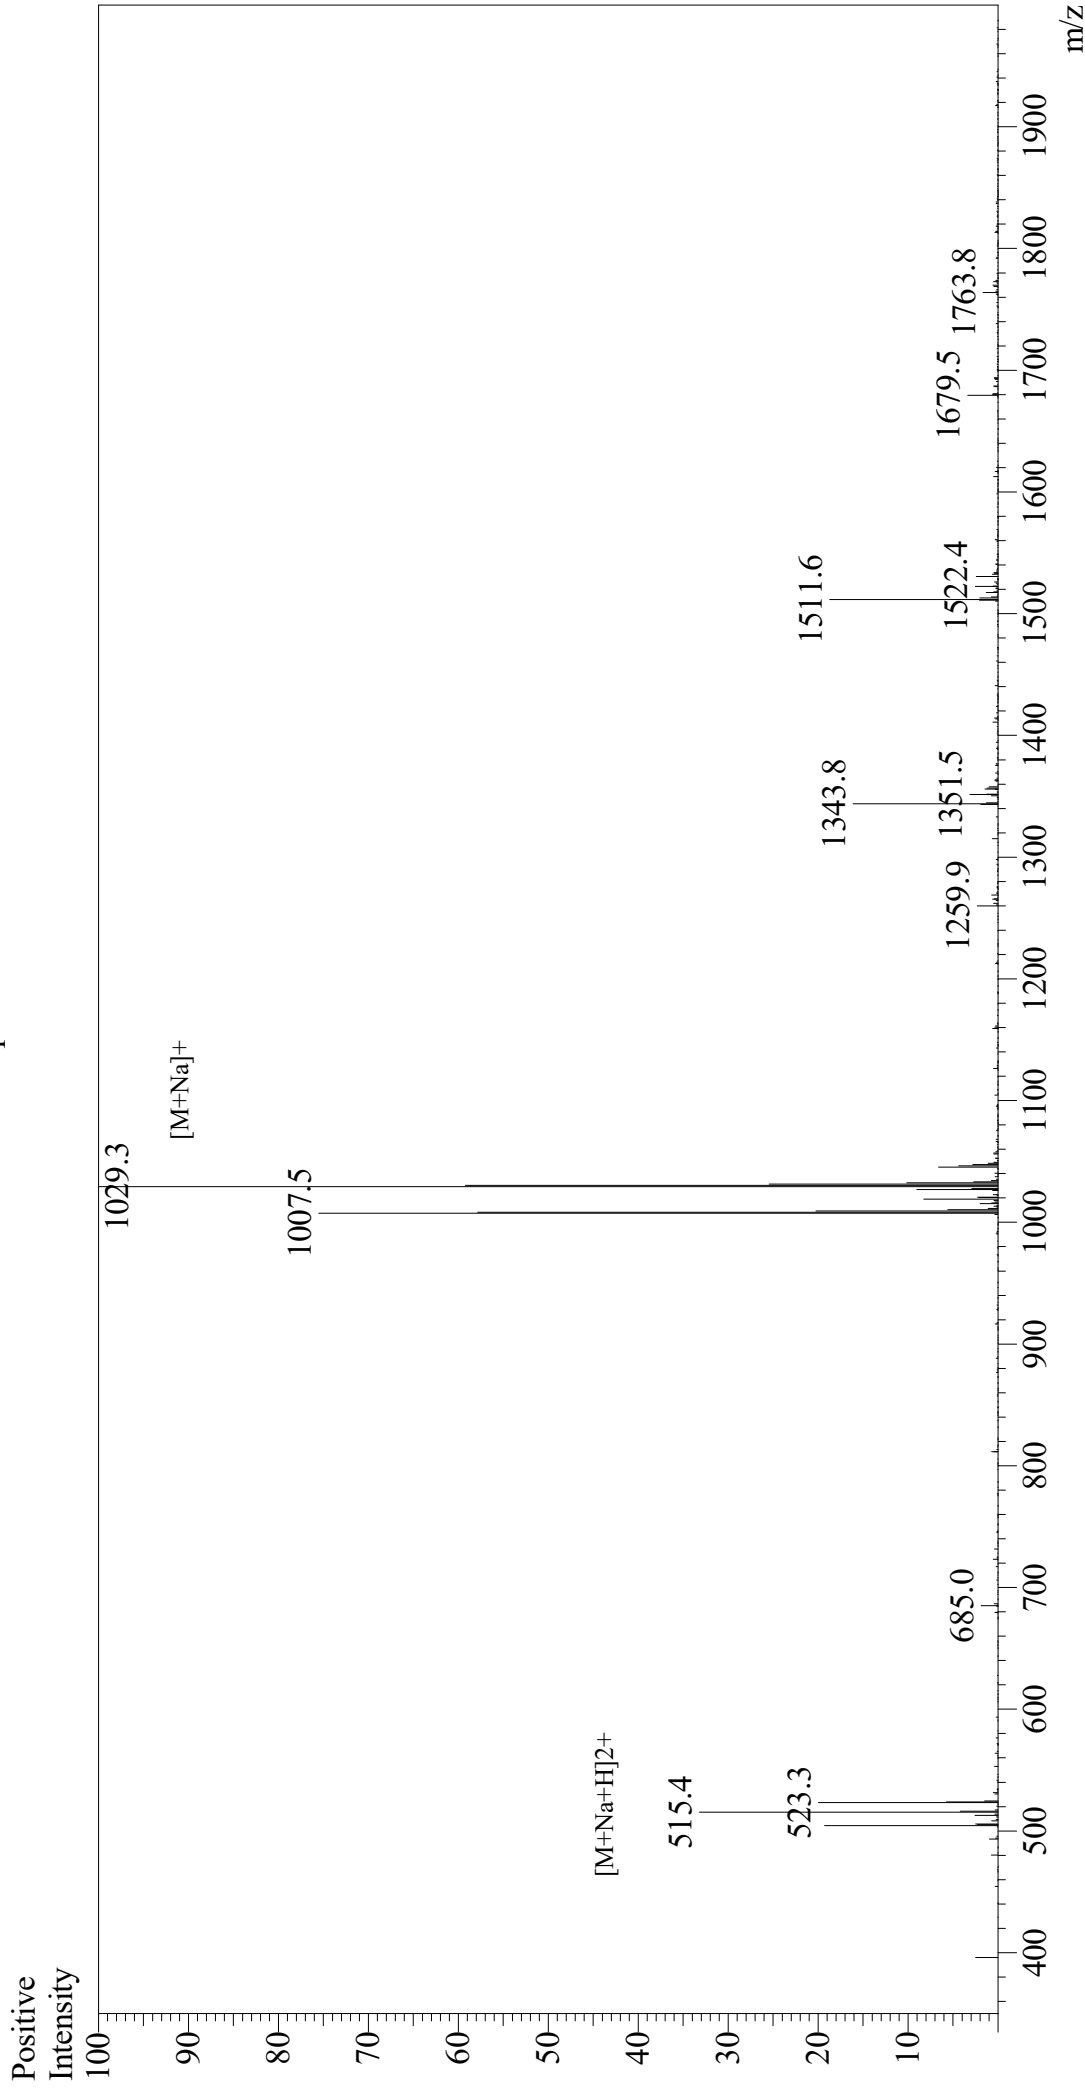

Sample Information
Month-Day Processed : 05/26/21
Time Processed : 7:53:08 AM
Injection Volume : 0.2
Sample Name : Oxytocin
Cat No : RP10407
Lot No : E0927821E
Theoretical MW : 1007.20
Observed MW : 1007.3

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH