

Sample Name :Peptide C105Y
 Cat No.: RP20382
 Lot No.: E4959119I
 Time Processed :10:45:59
 Month-Day-Year Processed :09/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 15 |
| 25.00 | Pumps | Pump A B.Conc | 75 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Conc | 95 |
| 31.01 | Pumps | Pump A B.Conc | 15 |
| 40.00 | Pumps | Pump A B.Conc | 15 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

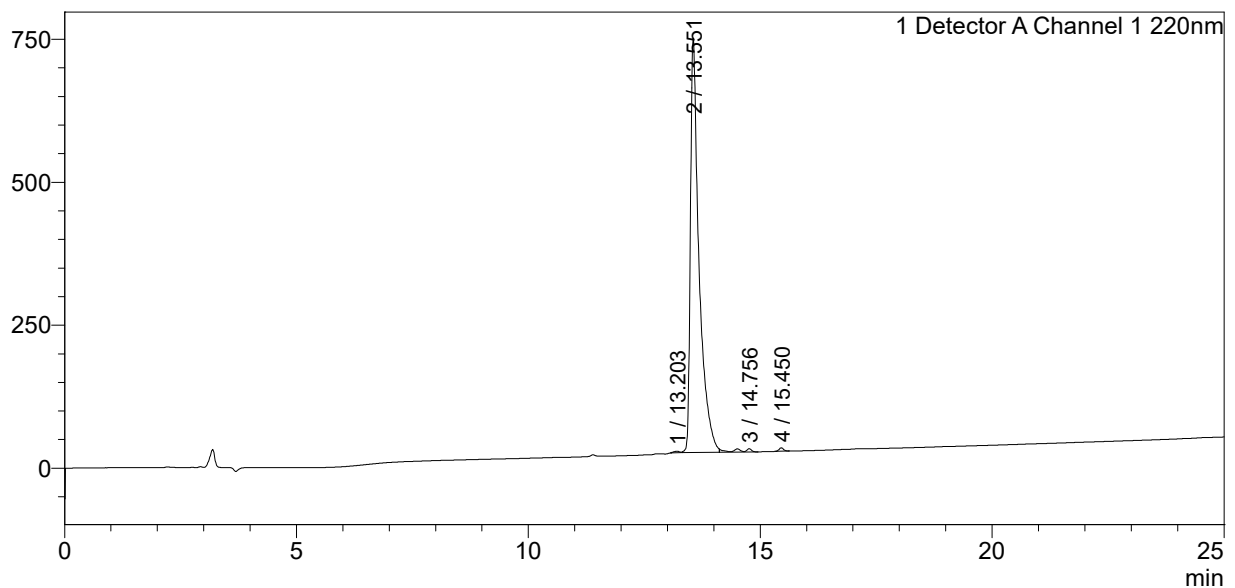

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 13.203 | 26493 | 2779 | 0.276 |
| 2 | 13.551 | 9415246 | 725300 | 97.986 |
| 3 | 14.756 | 127746 | 5836 | 1.329 |
| 4 | 15.450 | 39299 | 5928 | 0.409 |
| Total | | 9608785 | 739844 | 100.000 |