

Sample Name : Bacterial Sortase Substrate III, Abz/DNP
 Cat.No : RP20431
 Lot.No : E6692220B
 Time Processed: 21:23:44
 Year-Month-Day: 2020/2/23

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

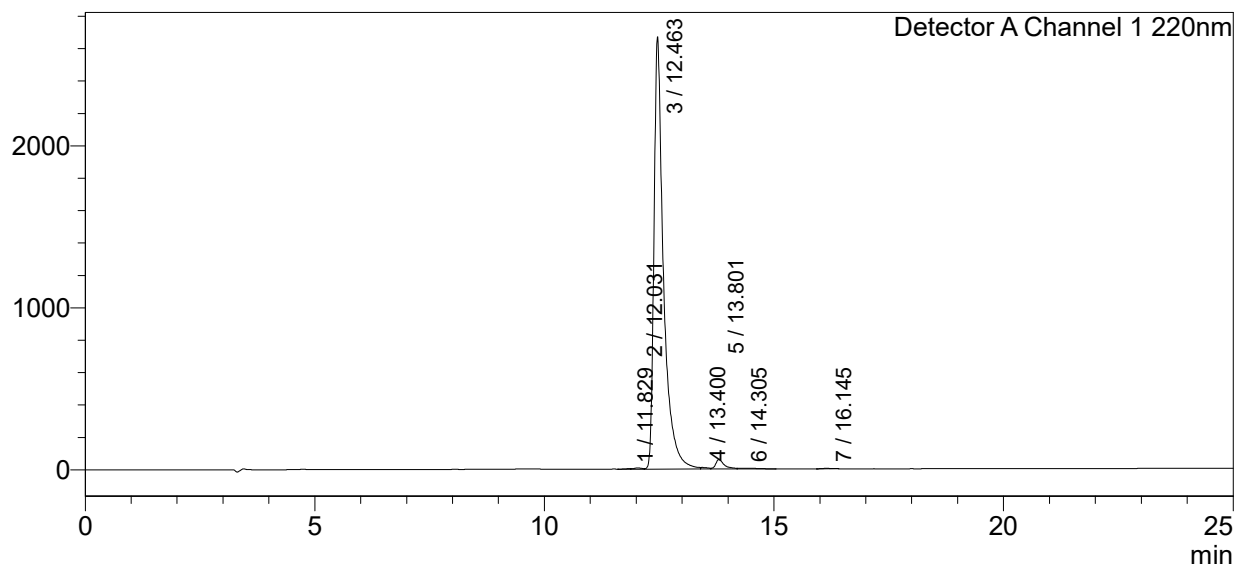

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.829	23430	2639	0.059
2	12.031	84063	7106	0.211
3	12.463	38702220	2668542	97.219
4	13.400	93727	9247	0.235
5	13.801	755959	58818	1.899
6	14.305	115996	4682	0.291
7	16.145	34002	2682	0.085
Total		39809398	2753717	100.000