


Mass Spectrum

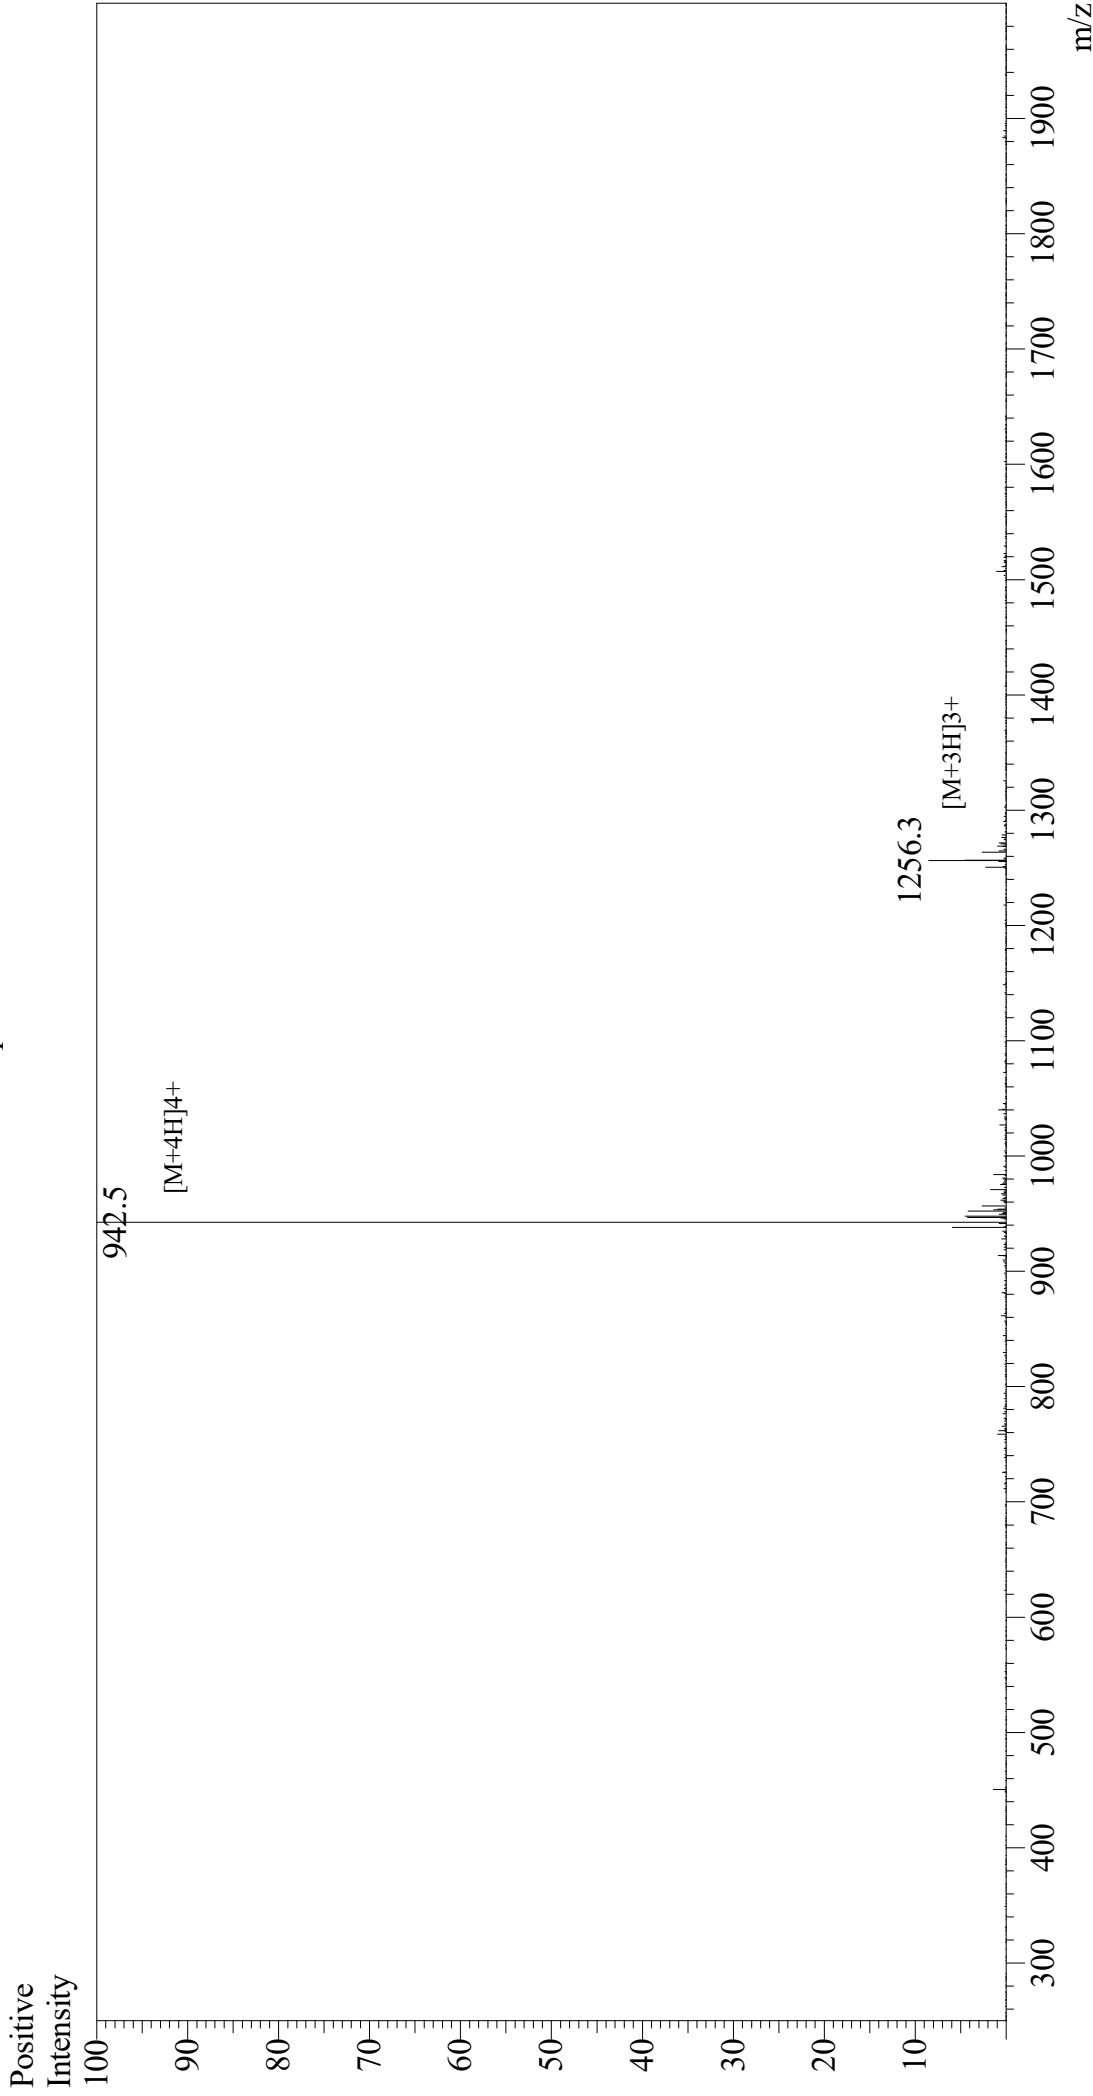

Sample Information		Interface		Equipment	
Month-Day Processed :	11/26/21	Nebulizing Gas Flow : 1.5L/min		: GK11010007	
Time Processed :	20:26:23	CDL Temp : 250		: +3.5 kV	
Injection Volume :	0.2	Block Temp : 200		: 5 L/min	
Sample Name :	Glucagon-Like Peptide (GLP) II, human			: 0.2 ml/min	
Cat No. :	RP10769			: 50% H ₂ O/50% MeOH	
Lot No. :	E3439221K				
Theoretical MW :	3766.20				
Observed MW :	3766.0				