

Sample Information

Sample Name :Flagelin22
 Cat. N.o :RP19986
 Lot. No. :PE6141901
 Time Processed :14:09:56
 Month-Day-Year Processed :02/03/2019

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

<<Pump>>
 Flow : 1.0000 mL/min


<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010508

Chromatogram

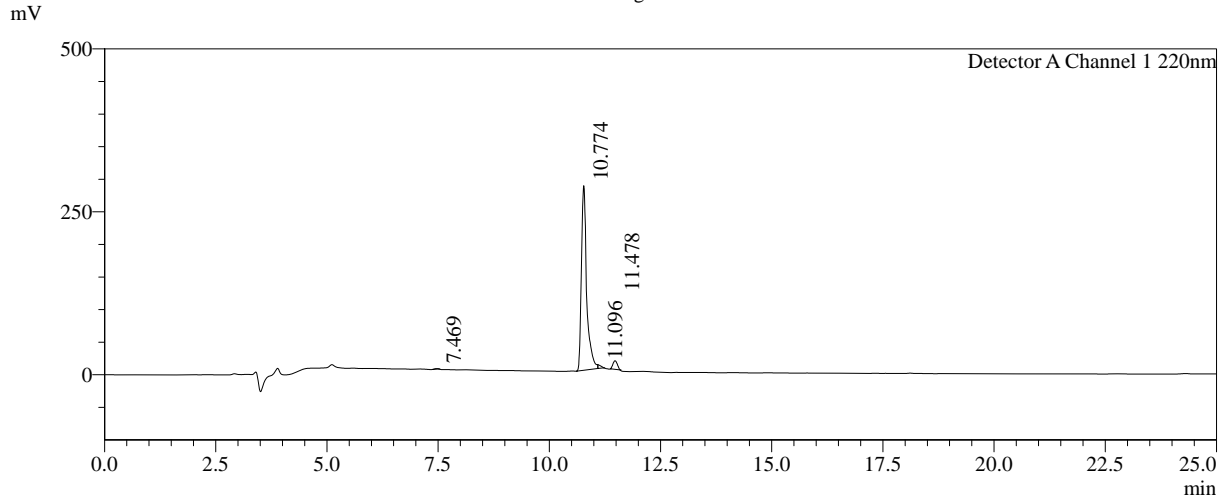

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Height	Area	Height%	Area%
1	7.469	821	4774	0.271	0.195
2	10.774	283228	2331066	93.491	95.143
3	11.096	5849	24129	1.931	0.985
4	11.478	13048	90087	4.307	3.677
Total		302946	2450055	100.000	100.000