

Sample Name :MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E9790319F
 Time Processed : 8:40:33
 Month-Day-Year Processed : 06/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	15	
31.00	Pumps	Pump A B.Conc	15	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

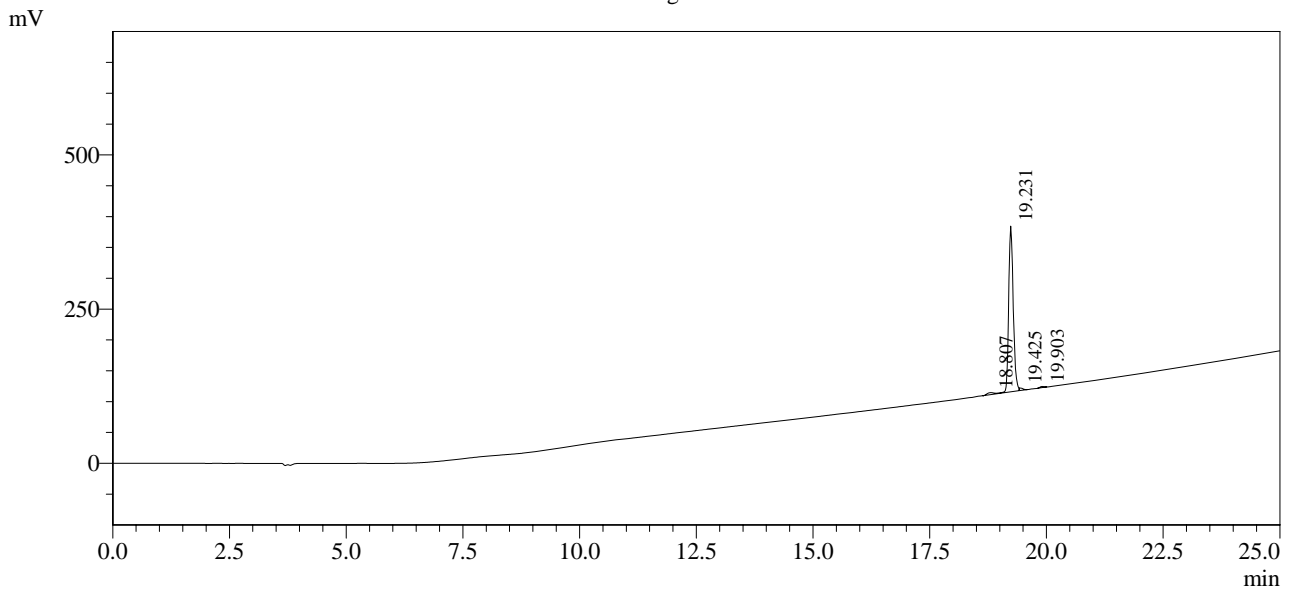

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.807	33879	3116	1.783
2	19.231	1835093	268847	96.559
3	19.425	20210	4170	1.063
4	19.903	11311	1922	0.595
Total		1900493	278055	100.000