

Sample Name :Neurotensin  
 Cat No. : RP10439  
 Lot No. : E5562619J  
 Time Processed : 22:32:32  
 Month-Day-Year Processed : 10/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

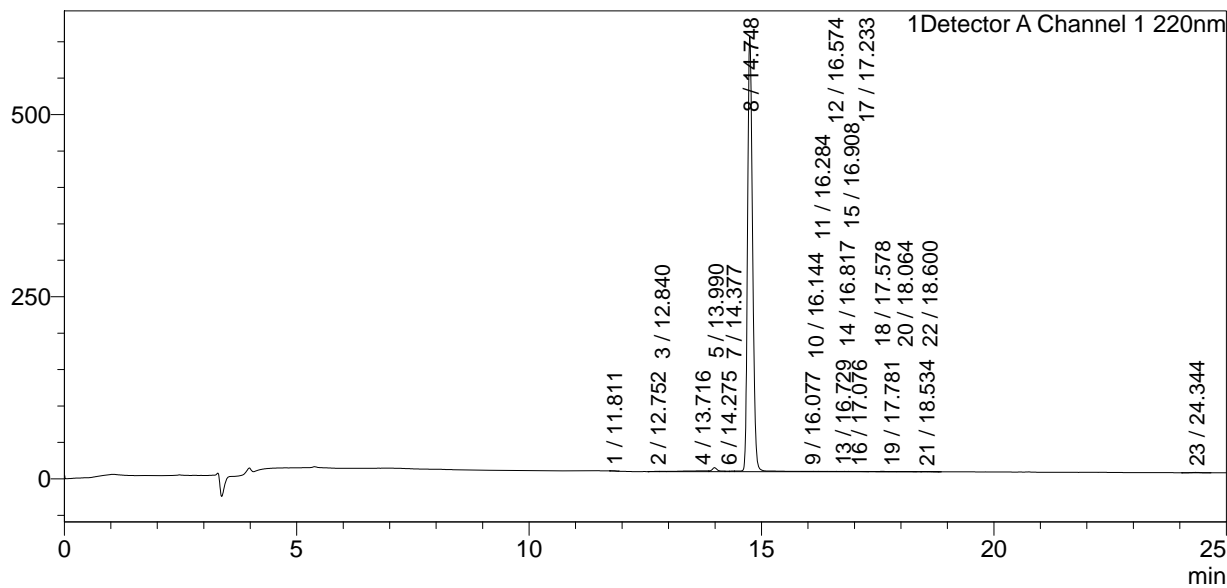

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.811	1750	338	0.037
2	12.752	3756	365	0.080
3	12.840	3053	354	0.065
4	13.716	43680	1206	0.935
5	13.990	47492	5565	1.017
6	14.275	4294	783	0.092
7	14.377	5224	822	0.112
8	14.748	4524359	597299	96.869
9	16.077	1448	188	0.031
10	16.144	1213	208	0.026
11	16.284	1932	210	0.041
12	16.574	1376	185	0.029
13	16.729	2151	259	0.046
14	16.817	1186	238	0.025
15	16.908	1738	203	0.037

Peak#	Ret. Time	Area	Height	Area%
16	17.076	1055	202	0.023
17	17.233	2244	217	0.048
18	17.578	4317	291	0.092
19	17.781	2076	236	0.044
20	18.064	5294	278	0.113
21	18.534	1809	242	0.039
22	18.600	2432	247	0.052
23	24.344	6701	553	0.143
Total		4670582	610489	100.000