

Sample Name : β -Amyloid (1-34)
 Cat No. : RP20140
 Lot No. : E5080320J
 Time Processed: 9:20:23 AM
 Month-Day-Year Processed :10/15/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

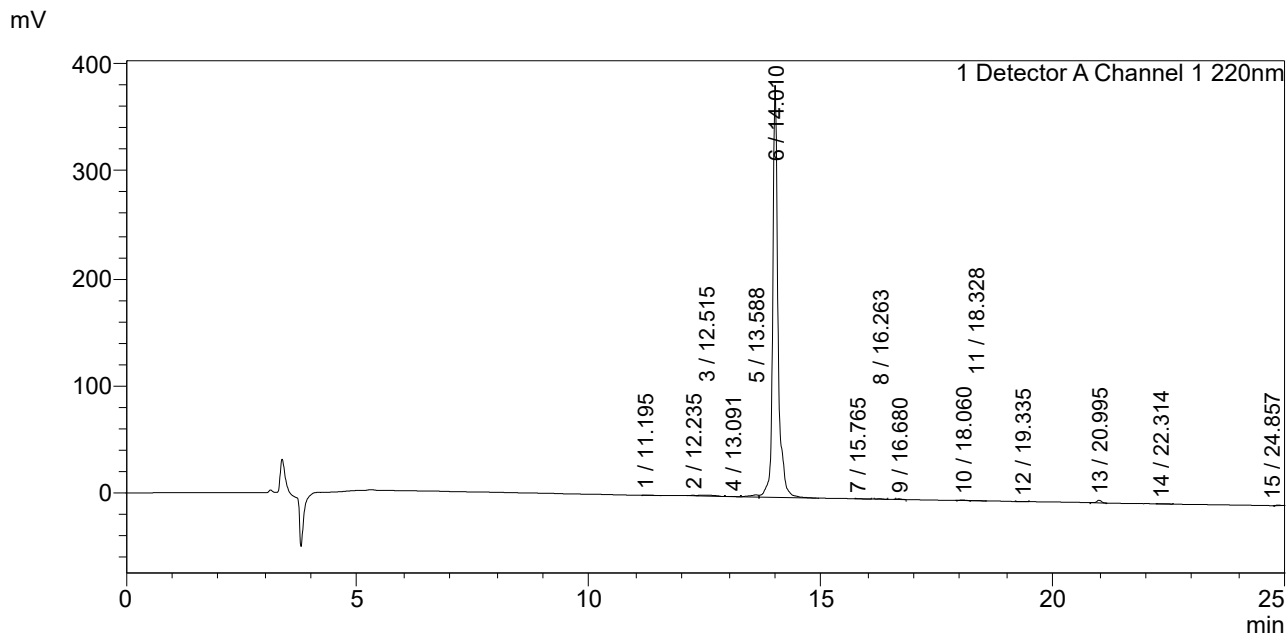

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.195	1701	127	0.054
2	12.235	3093	426	0.098
3	12.515	22000	907	0.696
4	13.091	2366	274	0.075
5	13.588	27787	2014	0.879
6	14.010	3070562	384465	97.081
7	15.765	1204	67	0.038
8	16.263	3011	468	0.095
9	16.680	3606	612	0.114
10	18.060	3503	377	0.111
11	18.328	1362	150	0.043
12	19.335	1103	127	0.035
13	20.995	16863	2537	0.533
14	22.314	1274	143	0.040
15	24.857	3445	491	0.109
Total		3162879	393184	100.000