

Sample Name :HA Peptide  
 Cat. No. :RP11735  
 Lot. No. :PE4131707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

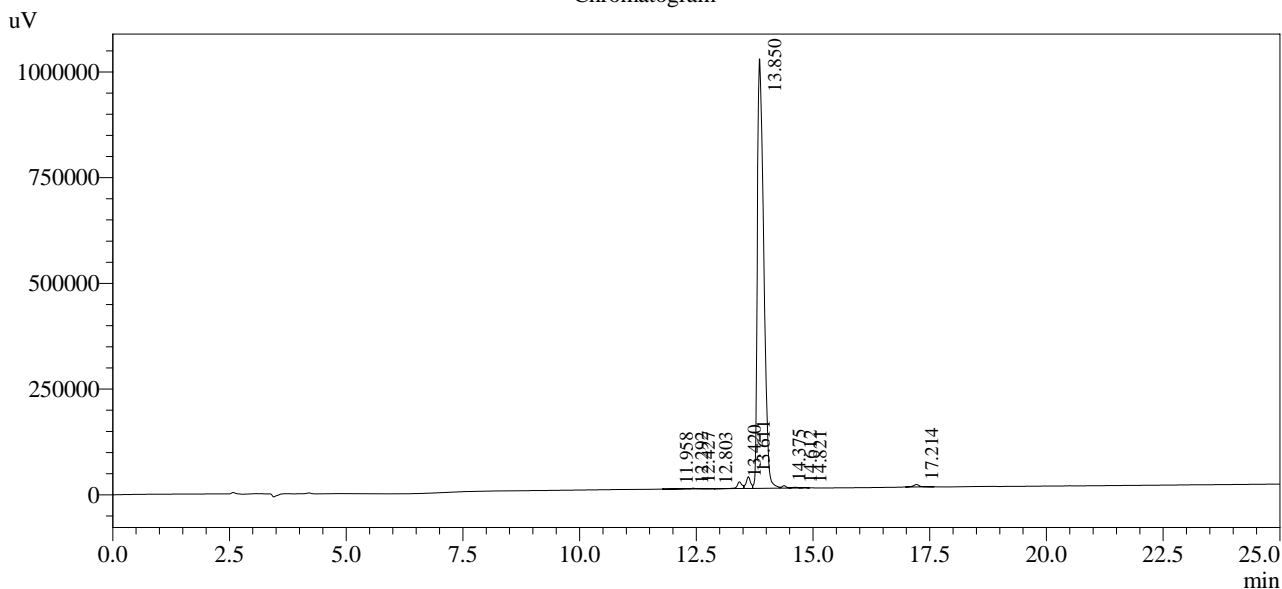

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.958	2391	292	0.024
2	12.292	5998	938	0.059
3	12.427	10435	1774	0.103
4	12.803	587	136	0.006
5	13.420	110761	15806	1.097
6	13.611	178868	27409	1.771
7	13.850	9681055	1015736	95.868
8	14.375	39018	5721	0.386
9	14.612	15312	1829	0.152
10	14.821	4873	975	0.048
11	17.214	49011	5589	0.485
Total		10098307	1076205	100.000