

Sample Name :MPG, HIV related
 Cat. No. : RP20335
 Lot. No. : E3923619F
 Time Processed : 5:44:25
 Month-Day-Year Processed :06/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

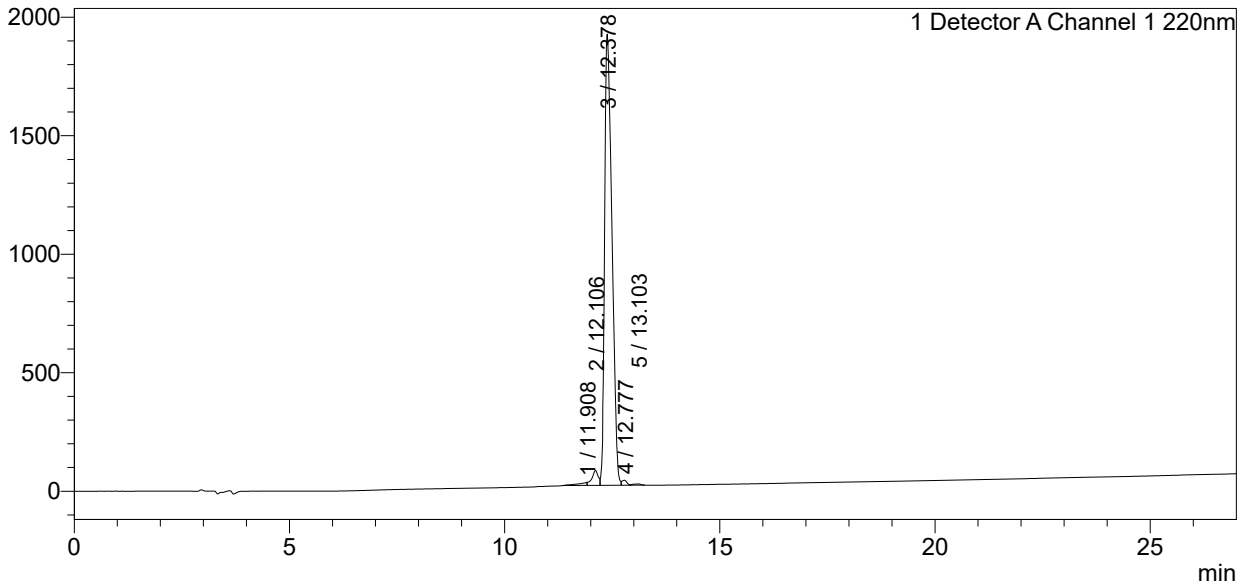

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.908	193010	12378	0.820
2	12.106	644656	63023	2.738
3	12.378	22482491	1904103	95.491
4	12.777	162087	21004	0.688
5	13.103	61968	4915	0.263
Total		23544212	2005423	100.000