

Sample Name :Angiotensin II (3-8), human
 Cat No. :RP11253
 Lot No. : E6527820J
 Time Processed : 1:29:18
 Month-Day-Year Processed : 10/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

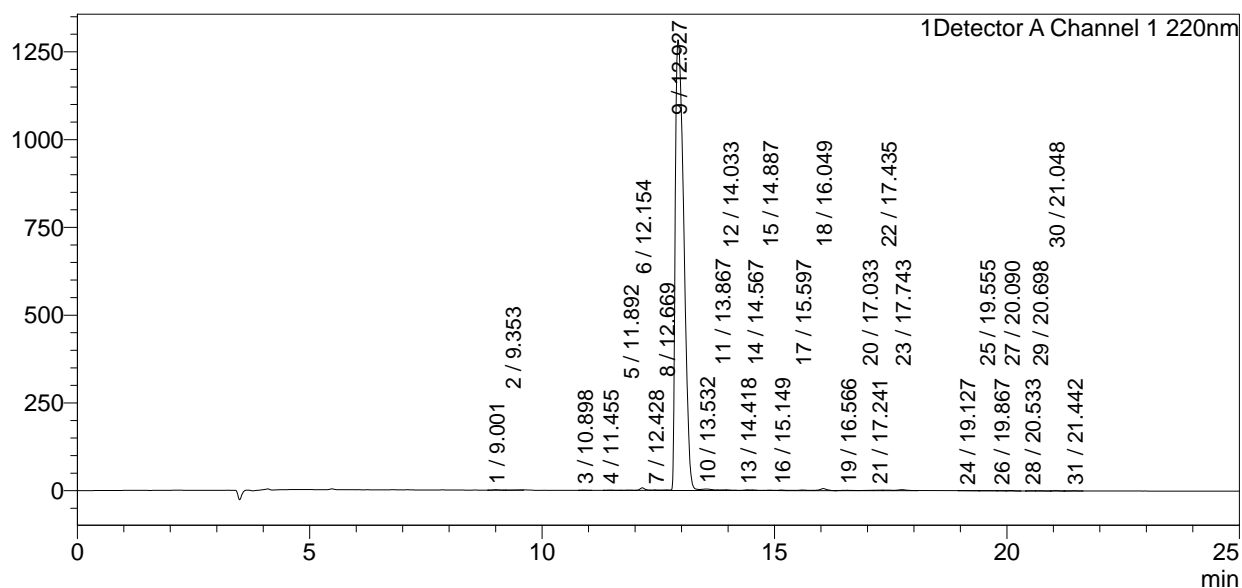

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.001	9878	1261	0.058
2	9.353	5552	720	0.033
3	10.898	2546	361	0.015
4	11.455	5280	499	0.031
5	11.892	6288	524	0.037
6	12.154	56589	7153	0.335
7	12.428	11516	1451	0.068
8	12.669	18994	1761	0.112
9	12.927	16372731	1281575	96.847
10	13.532	68868	4249	0.407
11	13.867	18188	1671	0.108
12	14.033	17552	1313	0.104
13	14.418	21656	2104	0.128
14	14.567	13973	1486	0.083
15	14.887	12950	1150	0.077

Peak#	Ret. Time	Area	Height	Area%
16	15.149	16040	1494	0.095
17	15.597	34788	1715	0.206
18	16.049	63531	5740	0.376
19	16.566	19105	1089	0.113
20	17.033	11807	876	0.070
21	17.241	13715	1426	0.081
22	17.435	16241	1614	0.096
23	17.743	35035	2642	0.207
24	19.127	6610	475	0.039
25	19.555	12092	1180	0.072
26	19.867	2874	352	0.017
27	20.090	10609	1326	0.063
28	20.533	3355	460	0.020
29	20.698	4359	566	0.026
30	21.048	7045	997	0.042
31	21.442	5941	610	0.035
Total		16905710	1329843	100.000