

Sample Name :G3-C12
 Cat No.: RP20329
 Lot No.: E7728220H
 Time Processed :3:35:31 PM
 Month-Day-Year Processed :08/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

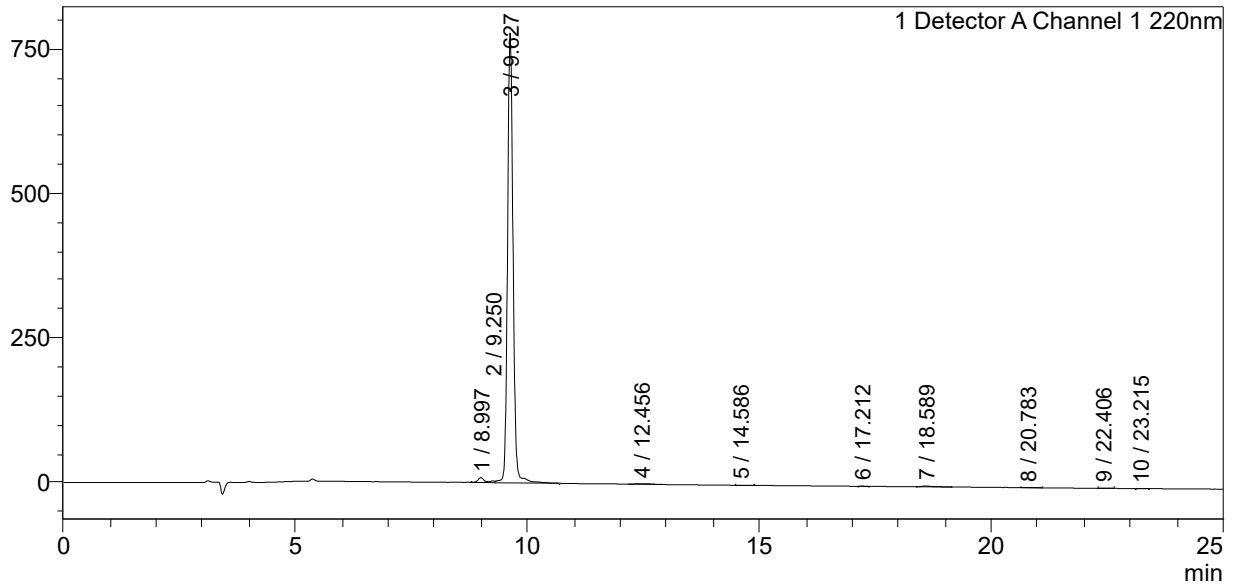

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.997	76116	8479	1.152
2	9.250	21324	2952	0.323
3	9.627	6460896	778270	97.762
4	12.456	18343	784	0.278
5	14.586	1415	86	0.021
6	17.212	1572	254	0.024
7	18.589	20937	1593	0.317
8	20.783	4603	340	0.070
9	22.406	2430	244	0.037
10	23.215	1173	165	0.018
Total		6608807	793166	100.000