

Sample Name :Competence-Stimulating Peptide-12261  
 Cat No. :RP20427  
 Lot No. :E4964619I  
 Time Processed : 4:01:22  
 Month-Day-Year Processed : 09/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

### <Chromatogram>

mV

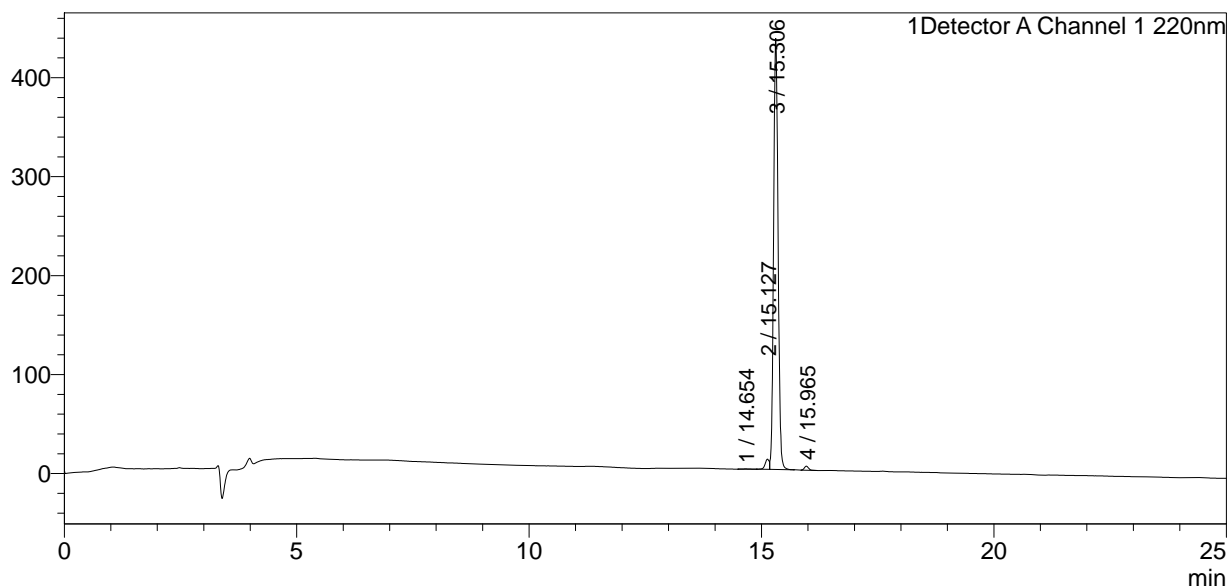

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.654	1760	235	0.059
2	15.127	63237	10313	2.106
3	15.306	2913107	435505	97.001
4	15.965	25068	4090	0.835
Total		3003172	450143	100.000