

Sample Name :OVA Peptide(257-264)
Cat. No. : RP10611
Lot. No. : PE4281811
Time Processed : 6:36:36
Month-Day-Year Processed : 11/07/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|--------------|-------|
| 0.01 | Pumps | Pump B Conc. | 5 |
| 25.00 | Pumps | Pump B Conc. | 65 |
| 25.01 | Pumps | Pump B Conc. | 95 |
| 27.00 | Pumps | Pump B Conc. | 95 |
| 27.01 | Pumps | Pump B Conc. | 5 |
| 32.00 | Pumps | Pump B Conc. | 5 |
| 32.01 | Controller | Stop | |

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

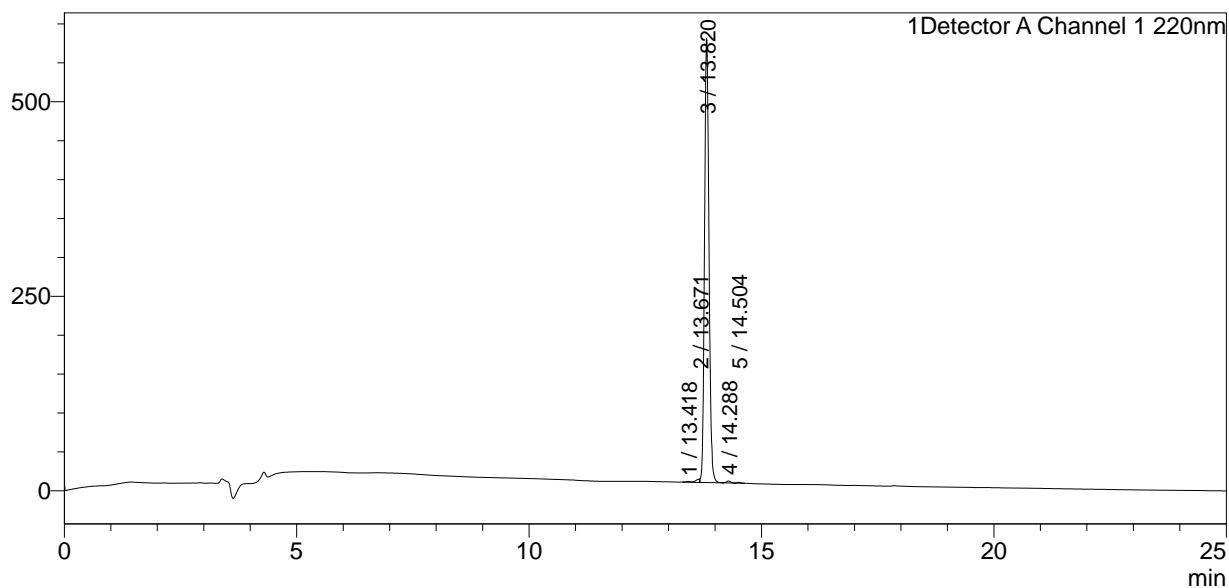

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 13.418 | 5566 | 815 | 0.145 |
| 2 | 13.671 | 24543 | 4245 | 0.638 |
| 3 | 13.820 | 3797231 | 570660 | 98.688 |
| 4 | 14.288 | 15008 | 2424 | 0.390 |
| 5 | 14.504 | 5358 | 1016 | 0.139 |
| Total | | 3847707 | 579160 | 100.000 |