

Sample Name :Peptide T
 Cat. No. : RP13035
 Lot. No. :E4671019I
 Time Processed :8:49:20
 Month-Day-Year Processed :09/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

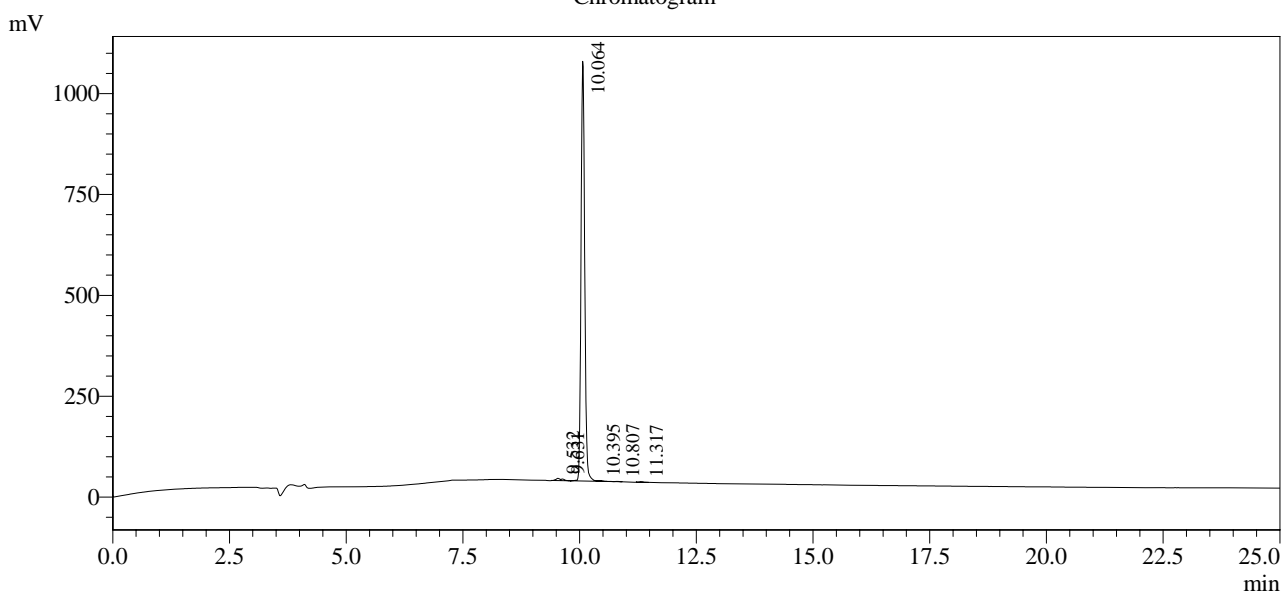

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.532	31672	5504	0.547
2	9.631	20654	3980	0.357
3	10.064	5719000	1040200	98.835
4	10.395	3484	706	0.060
5	10.807	2931	601	0.051
6	11.317	8682	1398	0.150
Total		5786422	1052390	100.000