

Sample Name :Astressin
 Cat. No. : RP10980
 Lot. No. :E0974819G
 Time Processed : 8:30:21
 Month-Day-Year Processed :07/22/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:SS-CM-0286

Chromatogram

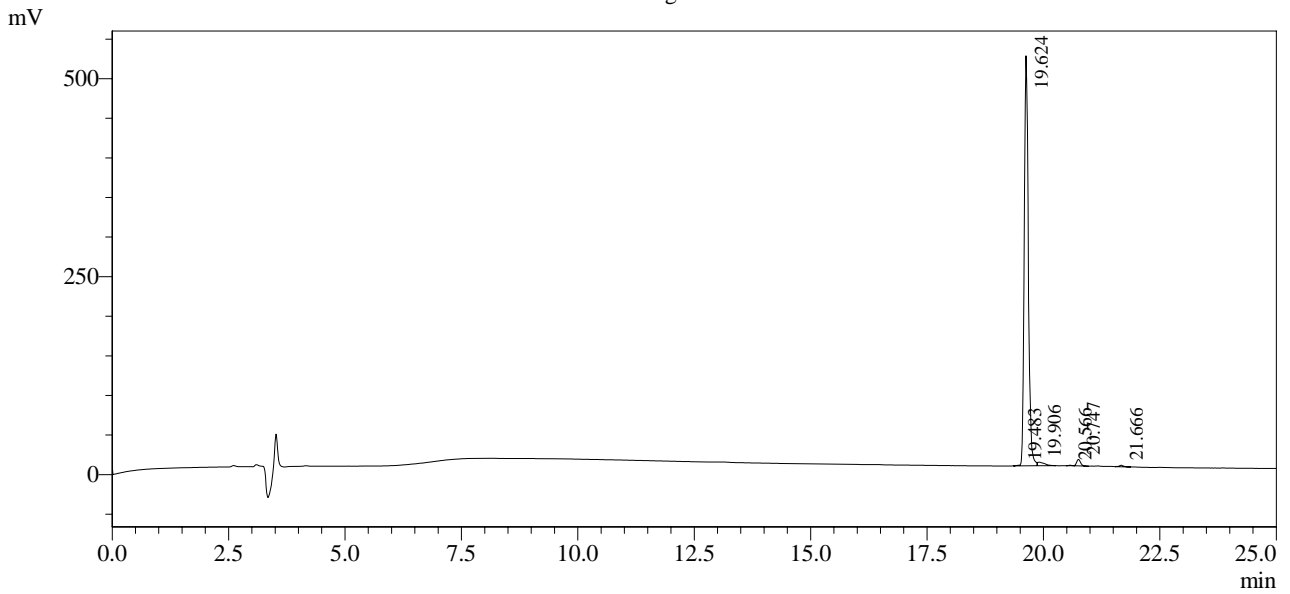

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	19.483	3654	834	0.112
2	19.624	3162555	517700	96.639
3	19.906	46248	4559	1.413
4	20.566	2916	633	0.089
5	20.747	45460	8067	1.389
6	21.666	11710	1871	0.358
Total		3272544	533663	100.000