


# Mass Spectrum

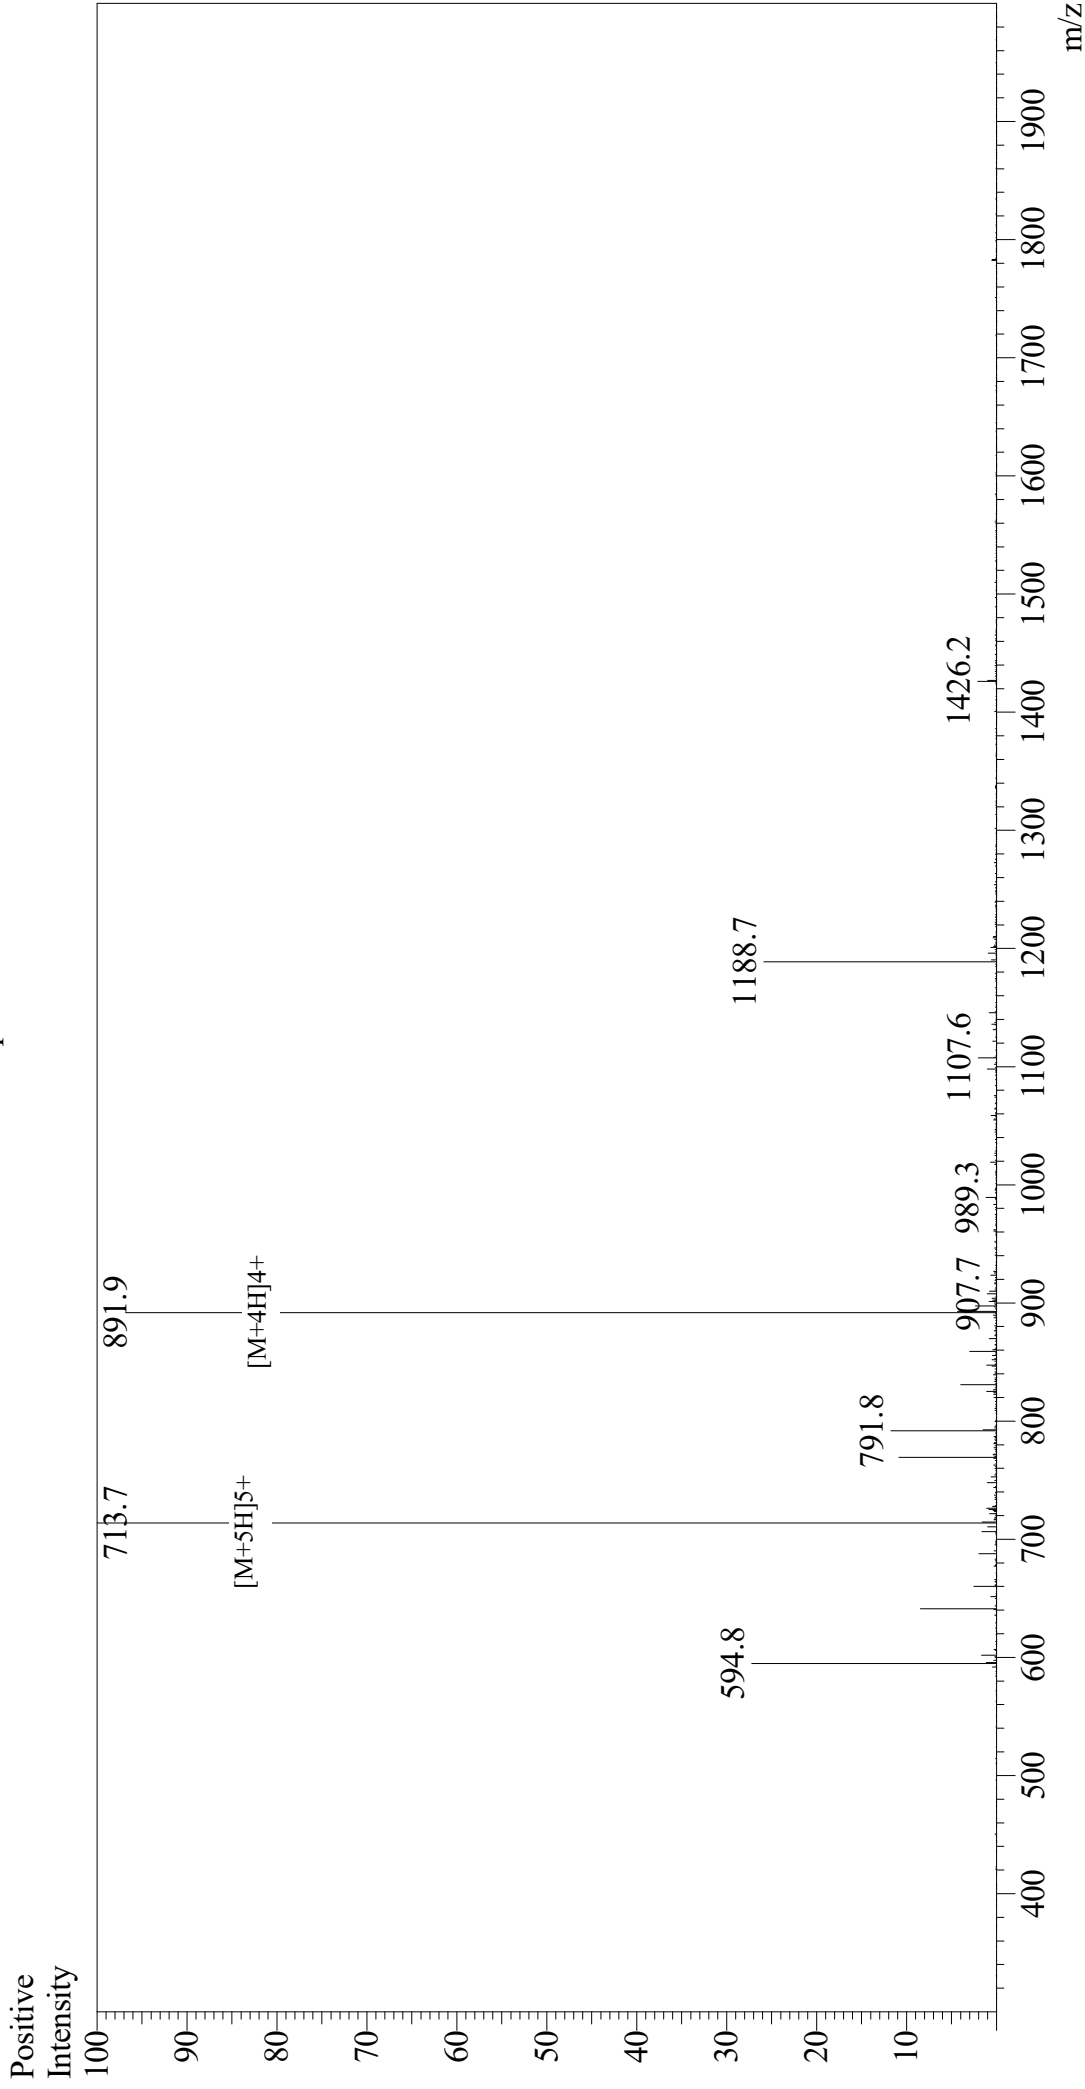

## Sample Information

Acquired by : Gary  
 Month-Day Processed : 07/21/19  
 Time Processed : 04:47:22 PM  
 Injection Volume : 0.3  
 Sample Name : Astressin  
 Cat. No. : RP10980  
 Lot. No. : E0974819G  
 Theoretical MW : 3563.16  
 Observed MW : 3563.5

## Interface

Interface : ESI  
 Nebulizing Gas Flow : 1.5L/min  
 CDL Temp : 250  
 Block Temp : 200

## Equipment

Equipment : GK11010007  
 Interface Bias : +4.5 kV  
 Drying Gas Flow : 5 L/min  
 T.Flow : 0.2 ml/min  
 B.conc : 50% H2O/50% MeOH