

Sample Name : AMARA peptide
 Cat. No. : RP20472
 Lot. No. : E9141019L
 Time Processed : 16:25:16
 Month-Day-Year Processed : 12/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

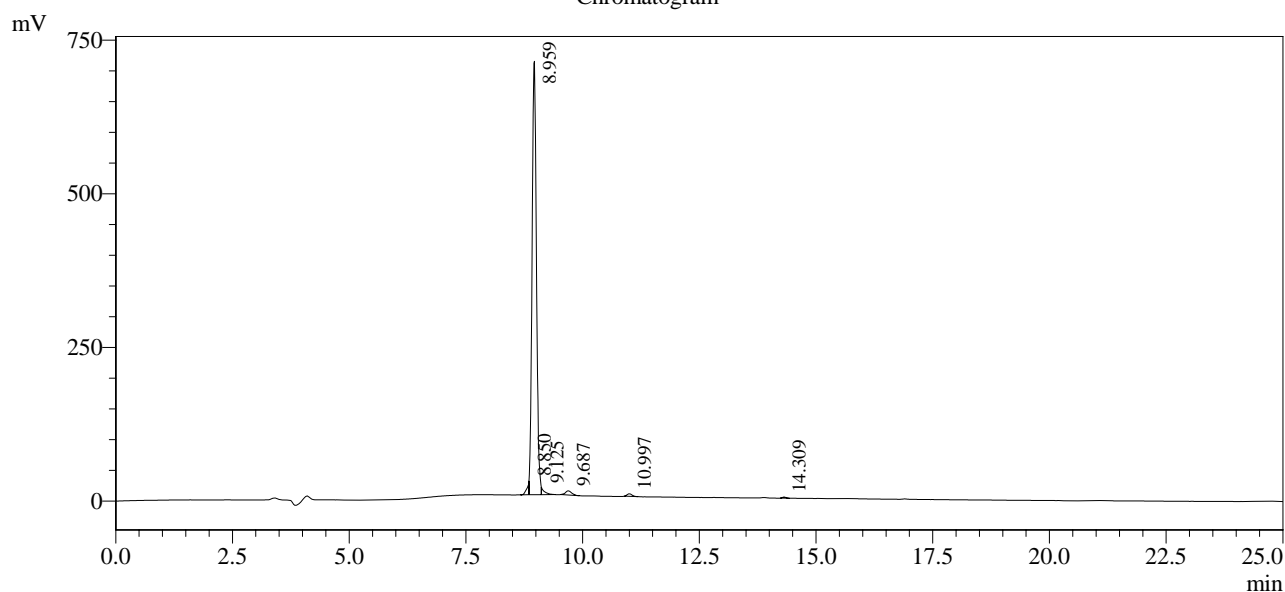

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.850	68144	22552	1.419
2	8.959	4585725	705379	95.477
3	9.125	48025	10459	1.000
4	9.687	63267	6698	1.317
5	10.997	29127	4035	0.606
6	14.309	8687	1710	0.181
Total		4802974	750834	100.000