

Sample Name :Shepherdin (79-87)  
 Cat No. :RP20410  
 Lot No. : E4942319I  
 Time Processed : 22:16:21  
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

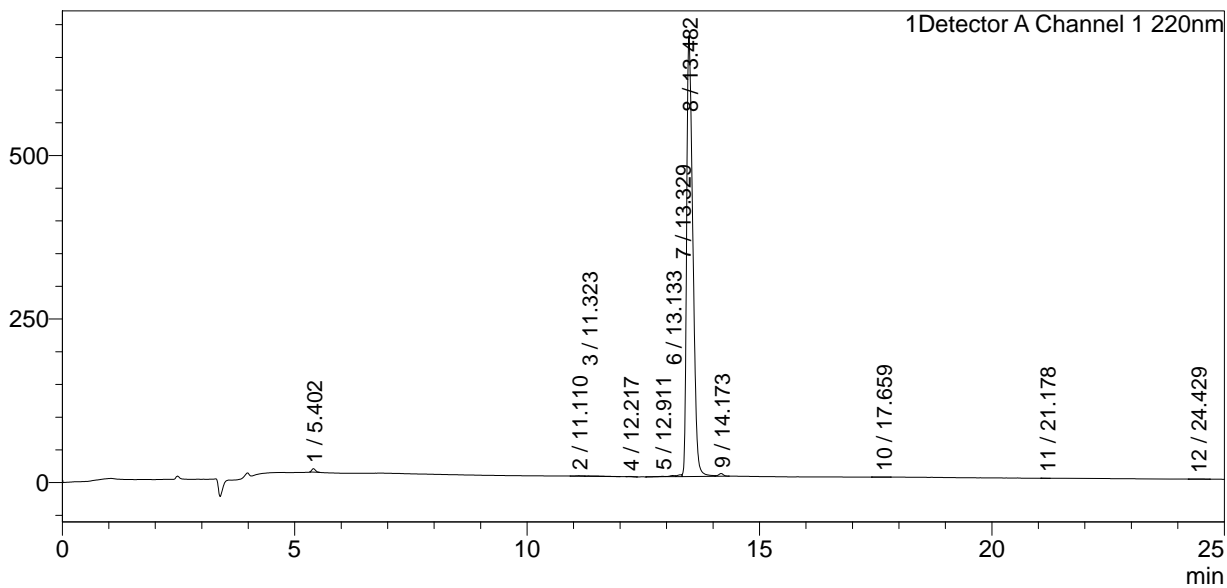

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.402	28394	5236	0.445
2	11.110	8028	685	0.126
3	11.323	14974	574	0.235
4	12.217	2868	478	0.045
5	12.911	7000	572	0.110
6	13.133	14258	1657	0.224
7	13.329	18089	2816	0.284
8	13.482	6240585	672598	97.913
9	14.173	30479	4116	0.478
10	17.659	2401	181	0.038
11	21.178	1181	139	0.019
12	24.429	5345	434	0.084
Total		6373602	689487	100.000